


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122122\
Data File : VU052466.D
Acq On : 21 Dec 2022 09:04
Operator : JC/MD
Sample : BFB182
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB182

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Dec 23 06:08:56 2022

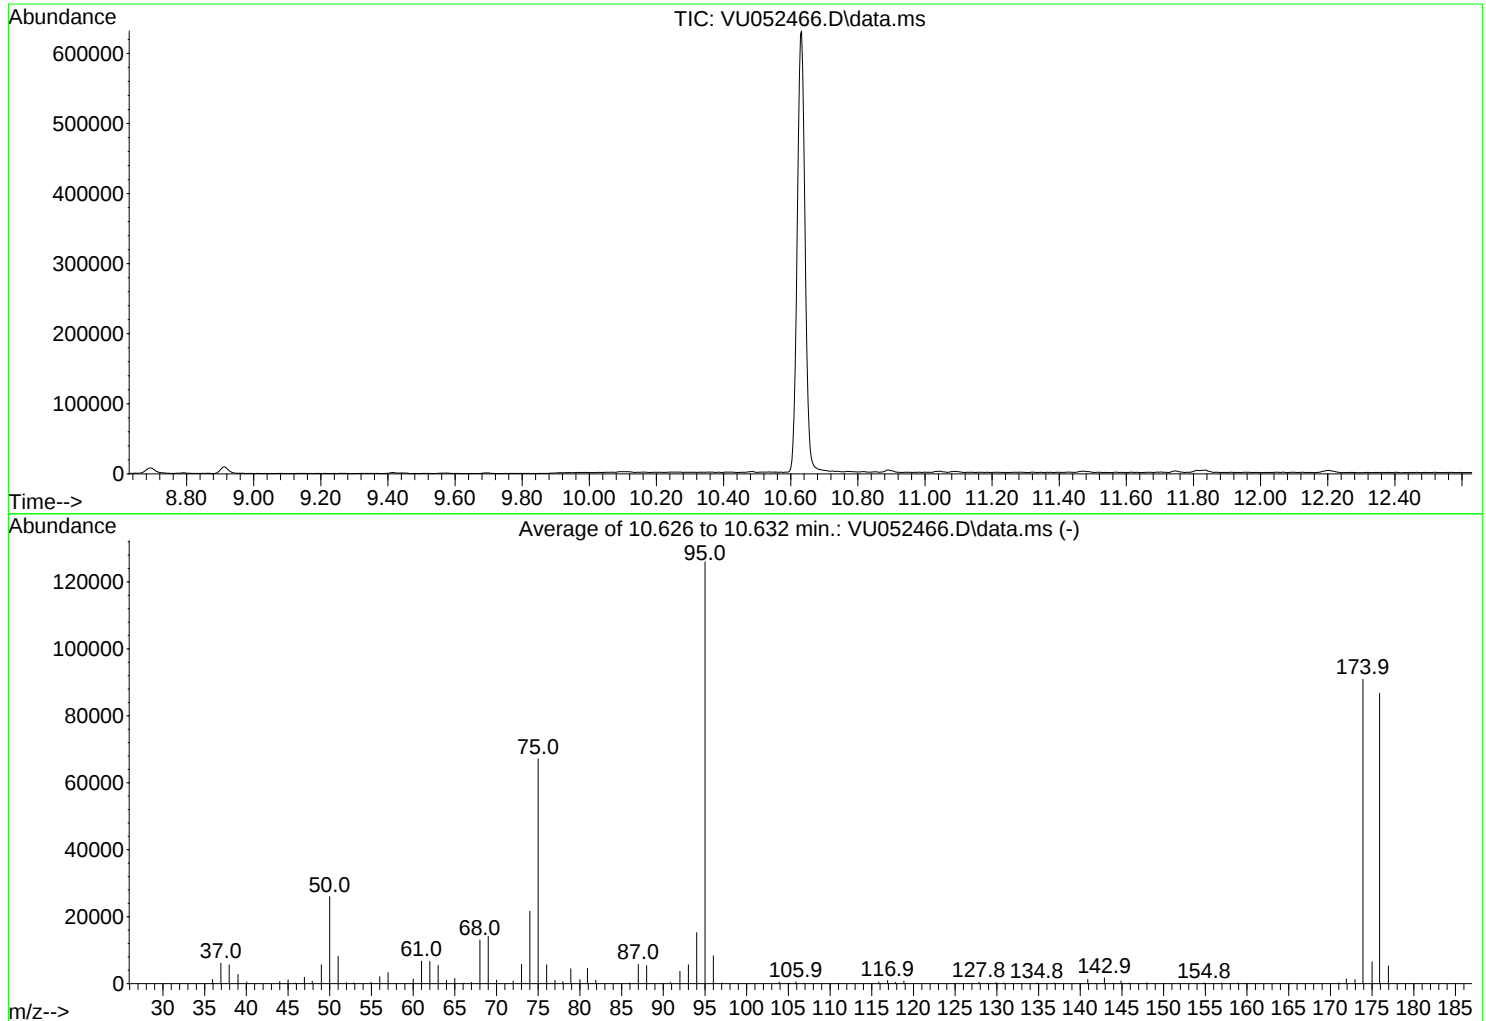

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	25984	PASS
75	95	30	80	53.3	67152	PASS
95	95	100	100	100.0	126008	PASS
96	95	5	9	6.6	8307	PASS
173	174	0.00	2	1.4	1237	PASS
174	95	50	120	72.2	90939	PASS
175	174	5	9	7.2	6526	PASS
176	174	95	101	95.3	86701	PASS
177	176	5	9	6.1	5312	PASS

m/z	Abundance
35.90	1249.0
36.90	180.0
37.90	356.0
39.80	265.0
44.00	447.0

Instrument :
MSVOA_U
ClientSampleId :
BFB182

m/z	Abundance
36.00	2558.0
37.00	6099.0
38.00	5627.0
39.00	2645.0
40.00	414.0
44.00	936.0
45.00	1209.0
45.90	172.0
46.90	1779.0
47.90	694.0
49.00	5252.0
50.00	24312.0
51.00	7747.0
52.00	343.0
52.90	235.0
55.00	403.0
56.00	1961.0
57.00	3234.0
60.00	1243.0
61.00	5973.0
62.00	6346.0
63.00	5079.0
64.00	987.0
65.00	1408.0
66.10	132.0
67.00	357.0
68.00	12490.0
69.00	13339.0
70.00	979.0
72.00	713.0
73.00	5503.0
74.00	20056.0
75.00	63232.0
76.00	5269.0
77.00	931.0
77.90	631.0
78.90	4267.0
80.00	1151.0
80.90	4376.0
81.90	909.0
86.00	214.0
87.00	5327.0
88.00	5149.0
90.80	400.0
92.00	3543.0
93.00	5391.0
94.00	13942.0
95.00	118640.0
96.00	7935.0
97.00	196.0
103.90	493.0
104.90	204.0
105.90	571.0
115.90	453.0
116.90	934.0
117.90	401.0
118.80	703.0
127.80	362.0
128.90	150.0
129.90	312.0
130.90	193.0
134.80	204.0
136.90	190.0
140.90	1227.0
141.80	121.0
142.90	1567.0
144.00	140.0
144.90	759.0
145.90	126.0
148.00	258.0
154.90	225.0
157.00	190.0
158.90	172.0
171.00	273.0
171.90	1380.0
173.00	1175.0
173.90	83424.0
175.00	6209.0
175.90	78880.0
177.00	4908.0

Instrument :
MSVOA_U
ClientSampleId :
BFB182

m/z	Abundance
36.00	2577.0
37.00	6524.0
38.00	6071.0
39.00	2856.0
40.10	482.0
44.00	1086.0
45.00	1200.0
45.90	179.0
47.00	1997.0
47.90	683.0
49.00	5712.0
50.00	26784.0
51.00	8533.0
52.00	368.0
52.80	264.0
55.00	382.0
56.00	2155.0
57.00	3367.0
60.00	1489.0
61.00	7062.0
62.00	6972.0
63.00	5696.0
64.00	996.0
65.00	1611.0
66.10	161.0
67.00	390.0
68.00	13427.0
69.00	14698.0
70.00	1133.0
72.00	831.0
73.00	5962.0
74.00	22096.0
75.00	69320.0
76.00	5783.0
77.00	1057.0
78.00	641.0
78.90	4551.0
80.00	1244.0
80.90	4656.0
81.90	1047.0
85.90	217.0
87.00	5906.0
88.00	5578.0
90.80	411.0
92.00	3857.0
93.00	5785.0
94.00	15703.0
95.00	129864.0
96.00	8583.0
97.10	232.0
103.90	514.0
105.10	244.0
105.90	583.0
106.80	114.0
110.80	113.0
115.80	494.0
116.90	1008.0
117.80	464.0
118.90	795.0
127.90	440.0
128.80	171.0
129.90	428.0
130.80	206.0
134.80	270.0
136.90	232.0
140.90	1331.0
141.90	122.0
142.90	1771.0
144.00	141.0
144.90	871.0
145.80	179.0
148.00	348.0
154.80	260.0
157.00	202.0
158.90	193.0
171.00	265.0
171.90	1487.0
173.00	1246.0
173.90	93640.0
175.00	6704.0
175.90	89104.0
177.00	5427.0

Instrument :
MSVOA_U
ClientSampleId :
BFB182

m/z	Abundance
36.00	2372.0
37.00	6269.0
38.00	6145.0
39.00	2805.0
40.10	482.0
44.00	1201.0
45.00	1069.0
45.90	187.0
47.00	2053.0
47.90	733.0
49.00	5931.0
50.00	26856.0
51.00	8456.0
52.00	364.0
52.80	216.0
54.90	394.0
56.00	2264.0
57.00	3367.0
58.00	129.0
60.00	1425.0
61.00	7158.0
62.00	6673.0
63.00	5605.0
64.00	898.0
65.00	1707.0
66.10	164.0
67.00	370.0
68.00	13213.0
69.00	14436.0
70.00	1034.0
72.00	895.0
73.00	5848.0
74.00	22640.0
75.00	68904.0
76.00	5898.0
77.00	1032.0
78.00	568.0
78.90	4524.0
80.00	1191.0
80.90	4632.0
81.90	1079.0
85.90	188.0
87.00	5986.0
88.00	5438.0
90.90	421.0
92.00	3650.0
93.00	5724.0
94.00	16052.0
95.00	129520.0
96.00	8404.0
97.10	238.0
103.90	498.0
105.10	260.0
105.90	583.0
106.80	154.0
110.90	112.0
115.80	512.0
116.90	930.0
117.80	462.0
118.90	834.0
127.90	467.0
128.80	181.0
129.90	475.0
130.80	220.0
134.80	335.0
136.90	210.0
140.90	1266.0
141.90	139.0
142.90	1855.0
143.90	164.0
144.90	840.0
145.90	245.0
148.00	371.0
148.90	104.0
151.80	101.0
154.80	289.0
156.80	206.0
158.90	177.0
171.00	215.0
171.90	1502.0
172.90	1290.0
173.90	95752.0
175.00	6664.0
175.90	92120.0
176.90	5600.0

Instrument :
MSVOA_U
ClientSampleId :
BFB182