

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122123\
 Data File : VU057169.D
 Acq On : 22 Dec 2023 05:42
 Operator : MD/SY
 Sample : 05912-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH3M6

Quant Time: Dec 22 07:10:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Dec 22 01:33:10 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	148097	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	141836	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	63997	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.596	65	71437	5.047	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	101.000%	
7) Chloroethane-d5	1.914	69	60119	5.160	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	103.200%	
11) 1,1-Dichloroethene-d2	2.563	65	30312	4.943	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	98.800%	
20) 2-Butanone-d5	4.637	46	131530	59.182	ug/L	0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	118.360%	
24) Chloroform-d	5.055	84	138750	5.076	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.600%	
26) 1,2-Dichloroethane-d4	5.695	65	68410	5.251	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	105.000%	
32) Benzene-d6	5.721	84	256273	5.268	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	105.400%	
36) 1,2-Dichloropropane-d6	6.685	67	75468	5.451	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	109.000%	
41) Toluene-d8	7.894	98	217169	4.890	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.800%	
43) trans-1,3-Dichloroprop...	8.174	79	28331	4.916	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	98.400%	
46) 2-Hexanone-d5	8.627	63	105029	53.529	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	107.060%	
56) 1,1,2,2-Tetrachloroeth...	10.750	84	56094	5.694	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	113.800%	
66) 1,2-Dichlorobenzene-d4	12.187	152	74020	5.375	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	107.600%	
Target Compounds					Qvalue	
42) Toluene	7.965	91	37407	0.785	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122123\
Data File : VU057169.D
Acq On : 22 Dec 2023 05:42
Operator : MD/SY
Sample : 05912-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH3M6

Quant Time: Dec 22 07:10:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Dec 22 01:33:10 2023
Response via : Initial Calibration

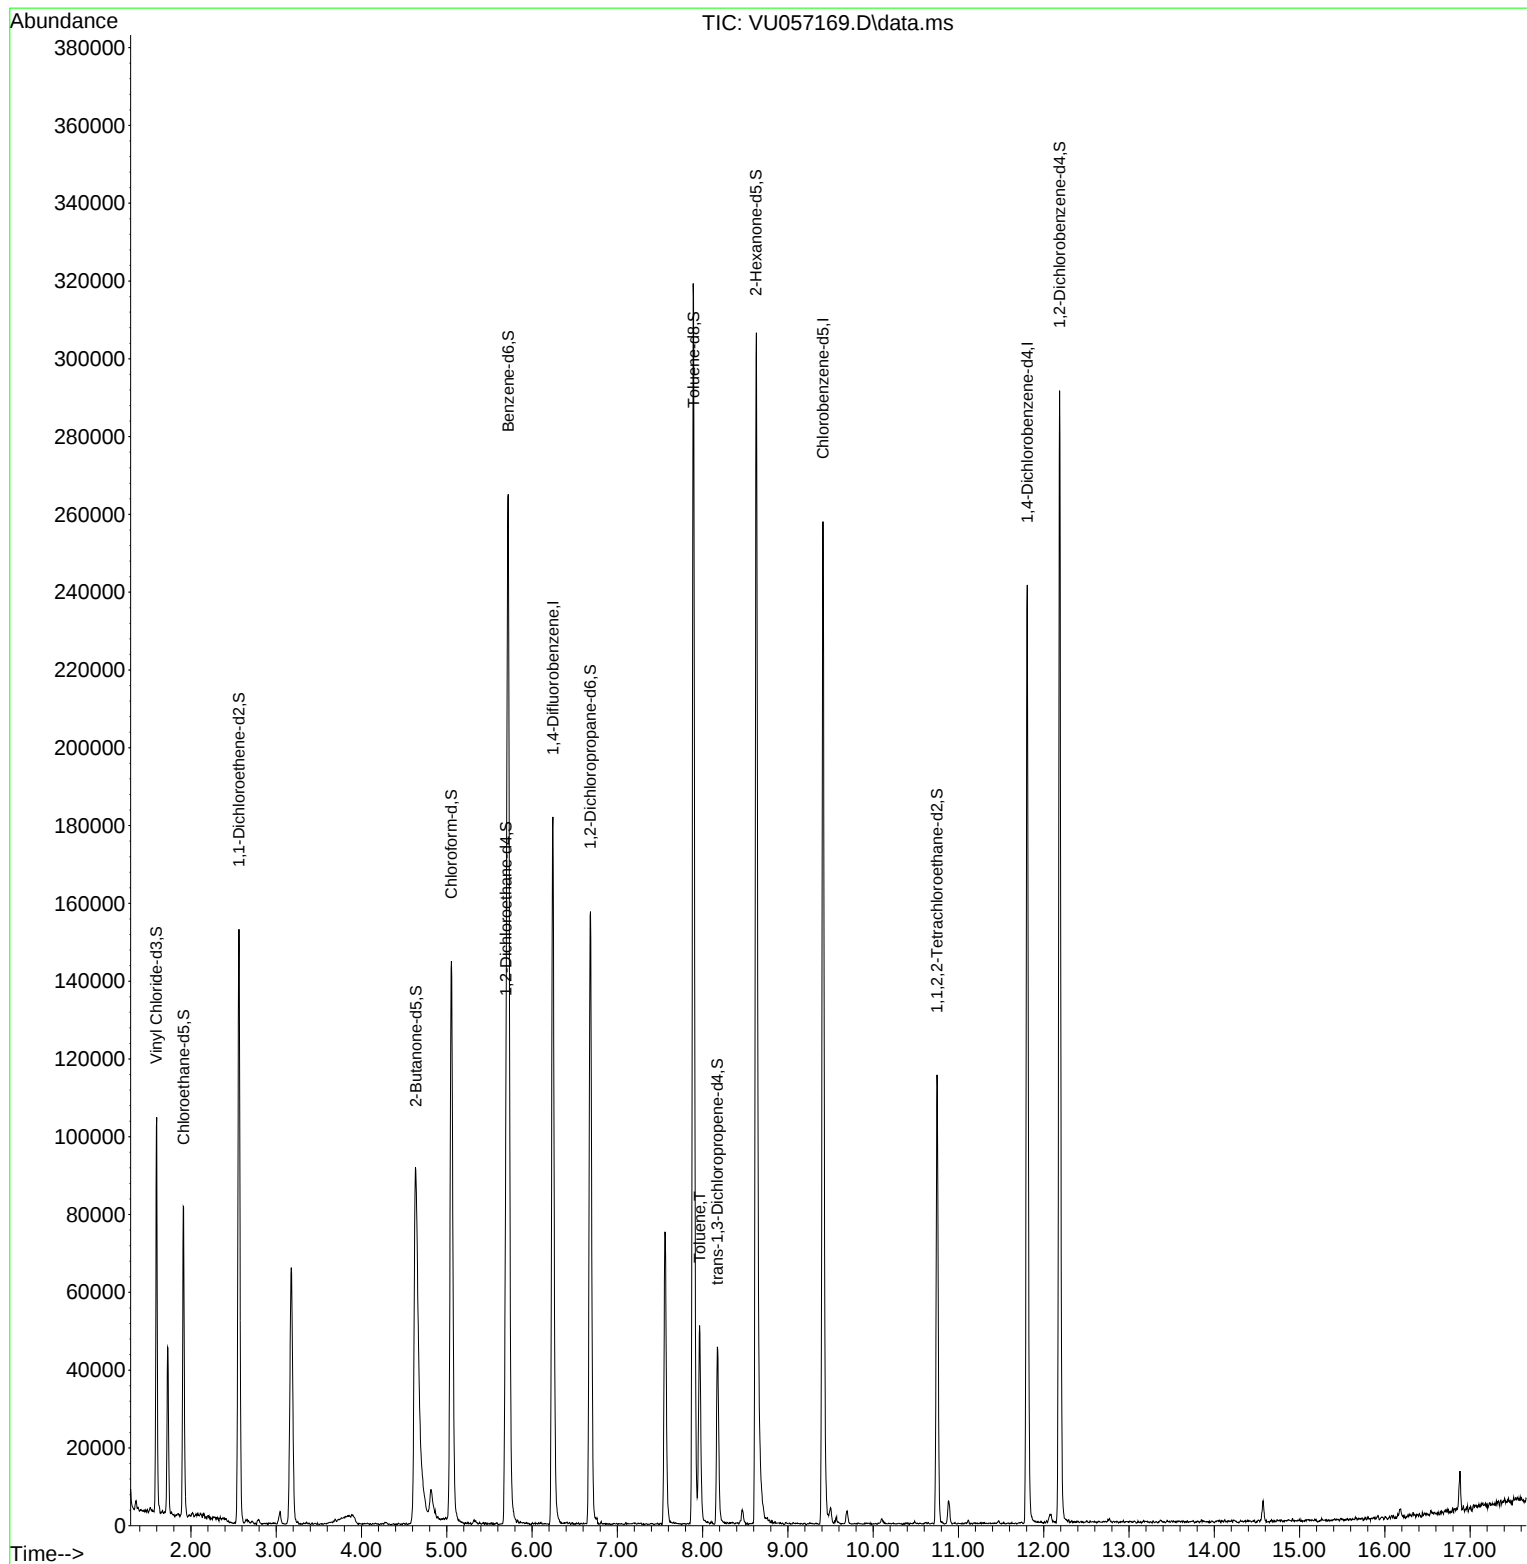

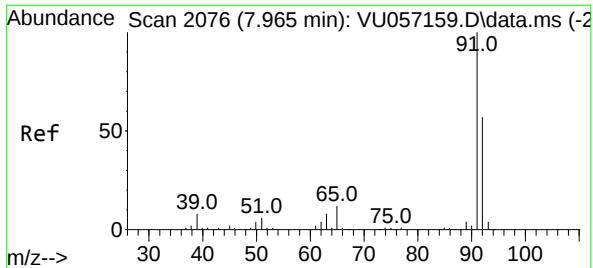

#42
Toluene
Concen: 0.785 ug/L
RT: 7.965 min Scan# 20
Delta R.T. -0.000 min
Lab File: VU057169.D
Acq: 22 Dec 2023 05:42

Instrument :
MSVOA_U
ClientSampleId :
BH3M6

Tgt Ion: 91 Resp: 37407
Ion Ratio Lower Upper
91 100
92 55.2 40.5 75.1

