

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122123\
 Data File : VU057143.D
 Acq On : 21 Dec 2023 18:49
 Operator : MD/SY
 Sample : 05866-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 F7C45

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU057143.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	85	96	107	rBV	101376	119523	17.19%	2.200%
2	1.911	185	193	208	rBV	82156	114390	16.45%	2.105%
3	2.563	380	396	414	rBV	163231	268395	38.60%	4.939%
4	4.624	1026	1037	1064	rBV	80398	216812	31.18%	3.990%
5	5.055	1156	1171	1197	rBV	146573	338153	48.63%	6.223%
6	5.515	1302	1314	1327	rBV3	8111	18672	2.69%	0.344%
7	5.721	1358	1378	1399	rBV2	265775	695329	100.00%	12.796%
8	6.242	1528	1540	1564	rBV	191330	375428	53.99%	6.909%
9	6.685	1665	1678	1702	rBV	165429	324688	46.70%	5.975%
10	7.560	1939	1950	1974	rBV2	77630	140521	20.21%	2.586%
11	7.894	2040	2054	2073	rBV	317180	566701	81.50%	10.429%
12	8.174	2128	2141	2162	rBV	47088	84151	12.10%	1.549%
13	8.467	2220	2232	2245	rBV2	4735	8551	1.23%	0.157%
14	8.628	2271	2282	2319	rBV	311364	599325	86.19%	11.029%
15	9.412	2512	2526	2545	rBV	266133	457421	65.78%	8.418%
16	10.750	2927	2942	2960	rBV	112088	184515	26.54%	3.396%
17	10.885	2973	2984	3000	rBV3	10105	16760	2.41%	0.308%
18	11.807	3259	3271	3287	rBV	256125	416841	59.95%	7.671%
19	12.187	3376	3389	3409	rBV	292494	487685	70.14%	8.975%




Sum of corrected areas: 5433861

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122123\
Data File : VU057143.D
Acq On : 21 Dec 2023 18:49
Operator : MD/SY
Sample : 05866-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

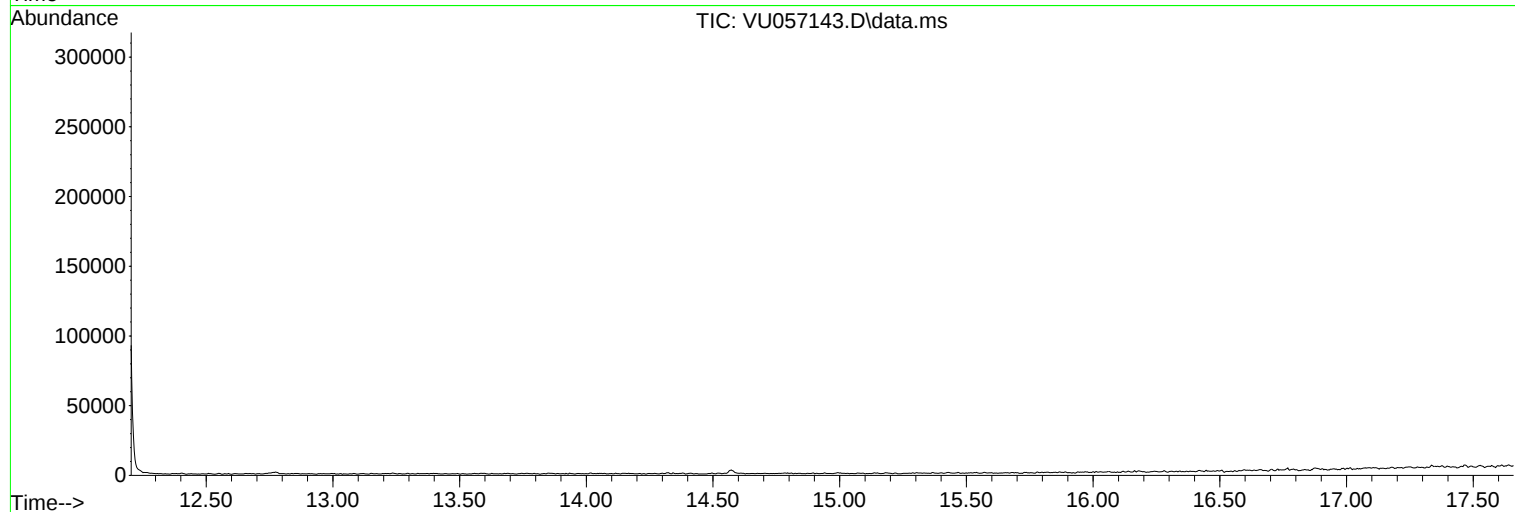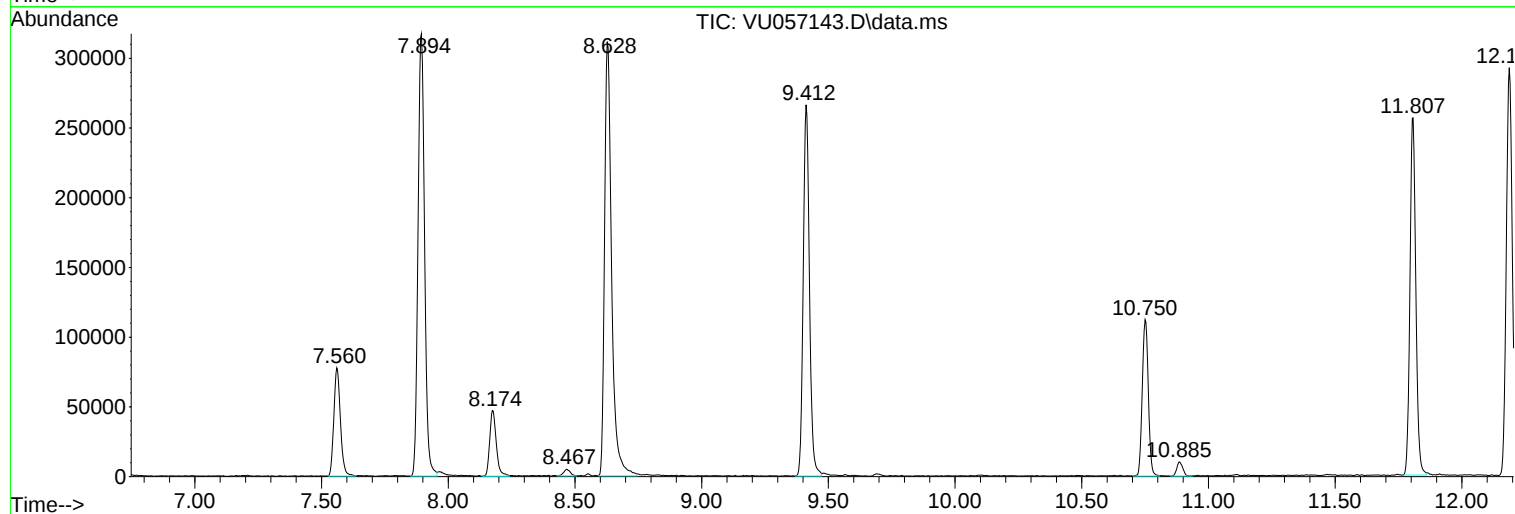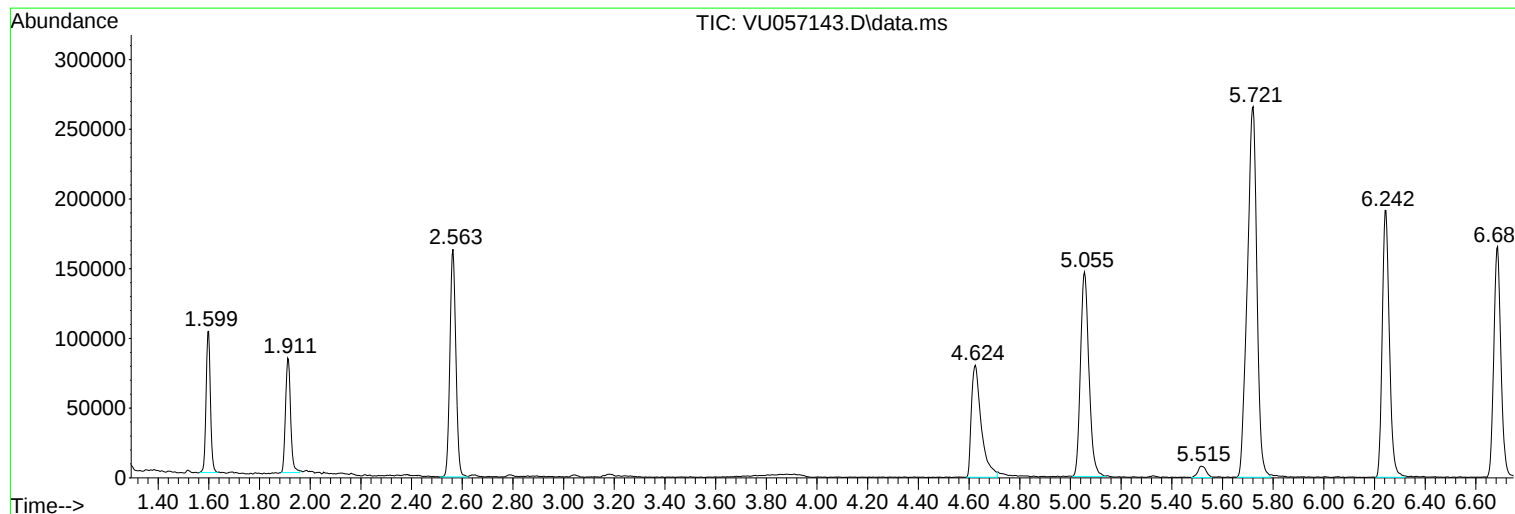

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122123\
Data File : VU057143.D
Acq On : 21 Dec 2023 18:49
Operator : MD/SY
Sample : 05866-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122123\
Data File : VU057143.D
Acq On : 21 Dec 2023 18:49
Operator : MD/SY
Sample : 05866-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
F7C45

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------