

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122123\
 Data File : VU057170.D
 Acq On : 22 Dec 2023 06:07
 Operator : MD/SY
 Sample : 05912-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH3M8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU057170.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.599	85	96	111	rVB	99375	117945	16.64%	2.169%
2	1.911	185	193	205	rBV	76324	103486	14.60%	1.903%
3	2.563	382	396	413	rBV	159213	260788	36.79%	4.795%
4	3.174	576	586	597	rBV3	3734	7157	1.01%	0.132%
5	4.624	1024	1037	1070	rBV2	82764	231310	32.63%	4.253%
6	5.055	1154	1171	1193	rBV	151904	335783	47.37%	6.174%
7	5.718	1357	1377	1397	rBV2	270205	708868	100.00%	13.035%
8	6.245	1527	1541	1565	rBV	184770	361231	50.96%	6.642%
9	6.682	1664	1677	1699	rBV2	169449	330106	46.57%	6.070%
10	7.560	1939	1950	1966	rBV2	78809	142311	20.08%	2.617%
11	7.891	2039	2053	2074	rBV	324430	571665	80.64%	10.512%
12	8.174	2130	2141	2155	rBV2	49481	83650	11.80%	1.538%
13	8.627	2271	2282	2317	rBV2	320098	626890	88.44%	11.527%
14	9.412	2513	2526	2546	rBV	261377	447696	63.16%	8.232%
15	10.750	2931	2942	2964	rVB2	115536	190653	26.90%	3.506%
16	10.888	2971	2985	2997	rVB2	6941	11184	1.58%	0.206%
17	11.807	3258	3271	3289	rBV	243879	396426	55.92%	7.290%
18	12.068	3343	3352	3368	rBV8	5773	14444	2.04%	0.266%
19	12.187	3376	3389	3416	rBV	295771	496707	70.07%	9.133%




Sum of corrected areas: 5438300

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122123\
Data File : VU057170.D
Acq On : 22 Dec 2023 06:07
Operator : MD/SY
Sample : 05912-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH3M8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

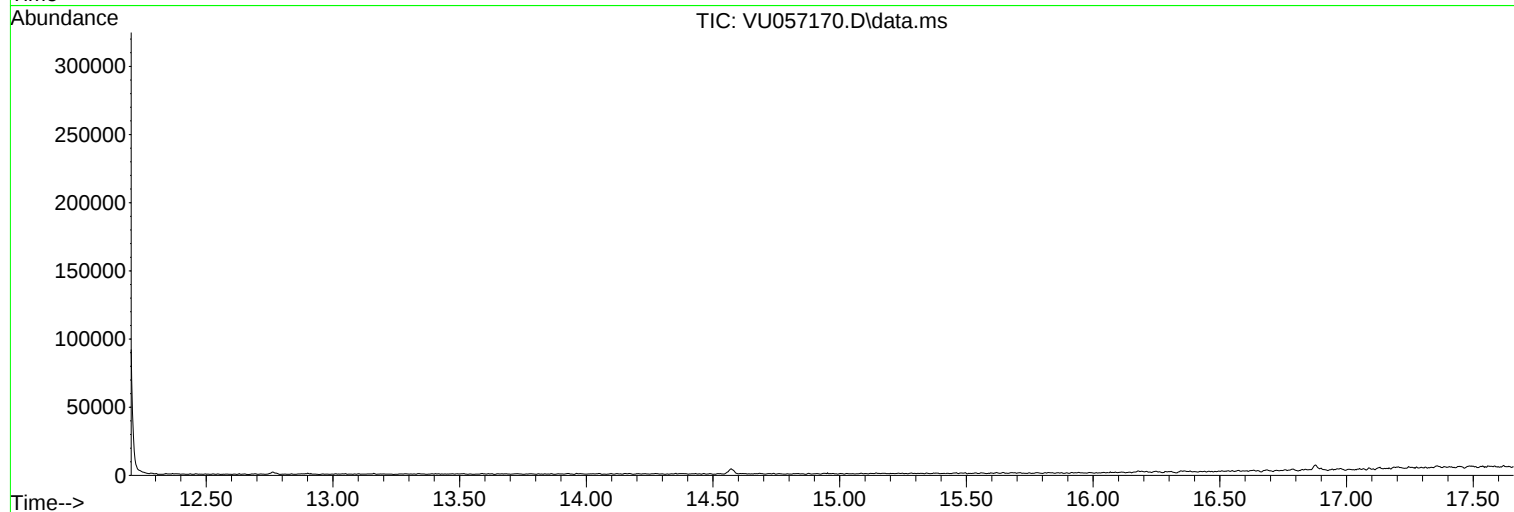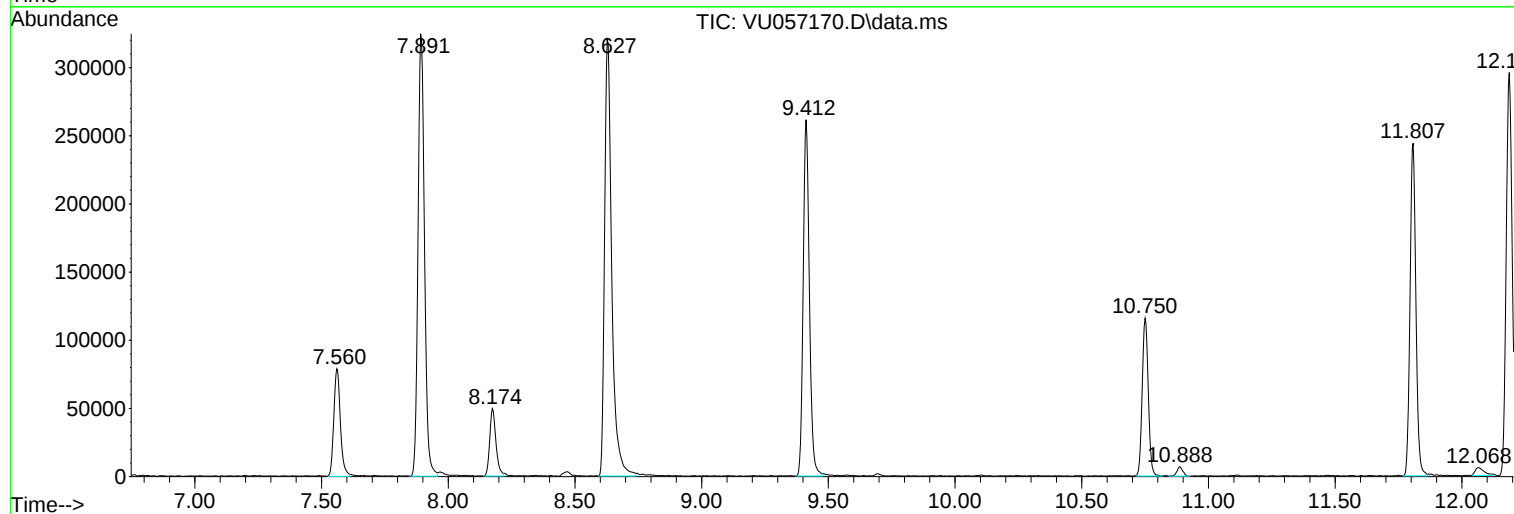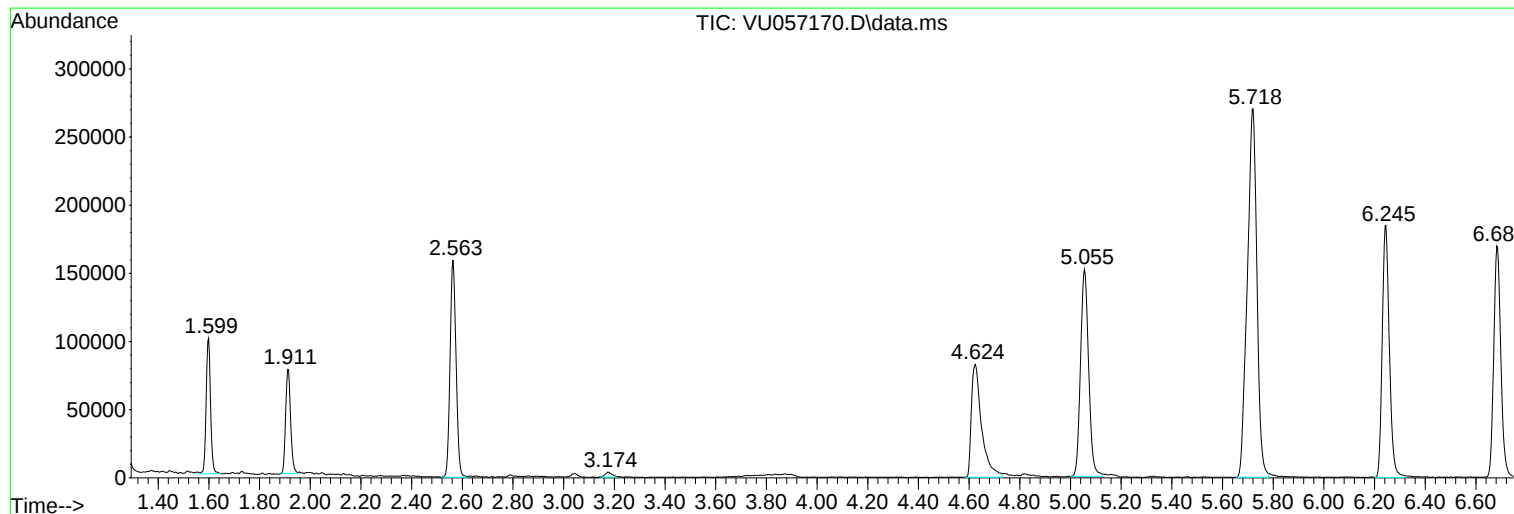

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122123\
Data File : VU057170.D
Acq On : 22 Dec 2023 06:07
Operator : MD/SY
Sample : 05912-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH3M8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122123\
Data File : VU057170.D
Acq On : 22 Dec 2023 06:07
Operator : MD/SY
Sample : 05912-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH3M8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------