

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122123\
 Data File : VU057176.D
 Acq On : 22 Dec 2023 08:31
 Operator : MD/SY
 Sample : 05912-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH3P5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU057176.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.460	50	53	62	rVB3	7303	8875	1.18%	0.146%
2	1.515	64	70	76	rVB4	6534	7862	1.04%	0.130%
3	1.599	88	96	111	rVB	106109	125295	16.60%	2.068%
4	1.914	184	194	208	rBV	73793	109732	14.54%	1.811%
5	2.557	381	394	413	rVB	165495	268883	35.63%	4.438%
6	3.039	532	544	564	rBV2	11653	26749	3.54%	0.442%
7	3.181	565	588	600	rBV3	15838	40405	5.35%	0.667%
8	4.634	1025	1040	1064	rBV	69027	217541	28.83%	3.591%
9	5.052	1155	1170	1193	rBV	154374	346722	45.94%	5.723%
10	5.718	1353	1377	1397	rBV2	294411	754689	100.00%	12.457%
11	6.242	1524	1540	1560	rBV	214549	414799	54.96%	6.847%
12	6.682	1663	1677	1696	rBV	172394	340831	45.16%	5.626%
13	7.560	1939	1950	1969	rBV	81240	148689	19.70%	2.454%
14	7.891	2037	2053	2073	rBV	349402	628866	83.33%	10.380%
15	8.177	2131	2142	2162	rBV2	49148	92931	12.31%	1.534%
16	8.470	2222	2233	2245	rVB3	4663	8240	1.09%	0.136%
17	8.656	2273	2291	2323	rBV	274364	658287	87.23%	10.866%
18	9.415	2513	2527	2548	rBV	289216	537690	71.25%	8.875%
19	9.692	2602	2613	2626	rBV2	14795	27670	3.67%	0.457%
20	10.100	2729	2740	2747	rBV4	4203	7579	1.00%	0.125%
21	10.759	2933	2945	2961	rBV	122859	202305	26.81%	3.339%
22	10.888	2973	2985	2996	rBV4	9709	15230	2.02%	0.251%
23	11.811	3257	3272	3293	rBV	304994	489672	64.88%	8.083%
24	12.071	3343	3353	3364	rBV5	9775	21927	2.91%	0.362%
25	12.190	3376	3390	3408	rBV	326734	536596	71.10%	8.857%
26	14.572	4123	4131	4143	rVB3	5070	8095	1.07%	0.134%
27	16.180	4621	4631	4641	rBV4	7471	12028	1.59%	0.199%




Sum of corrected areas: 6058188

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122123\
Data File : VU057176.D
Acq On : 22 Dec 2023 08:31
Operator : MD/SY
Sample : 05912-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH3P5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

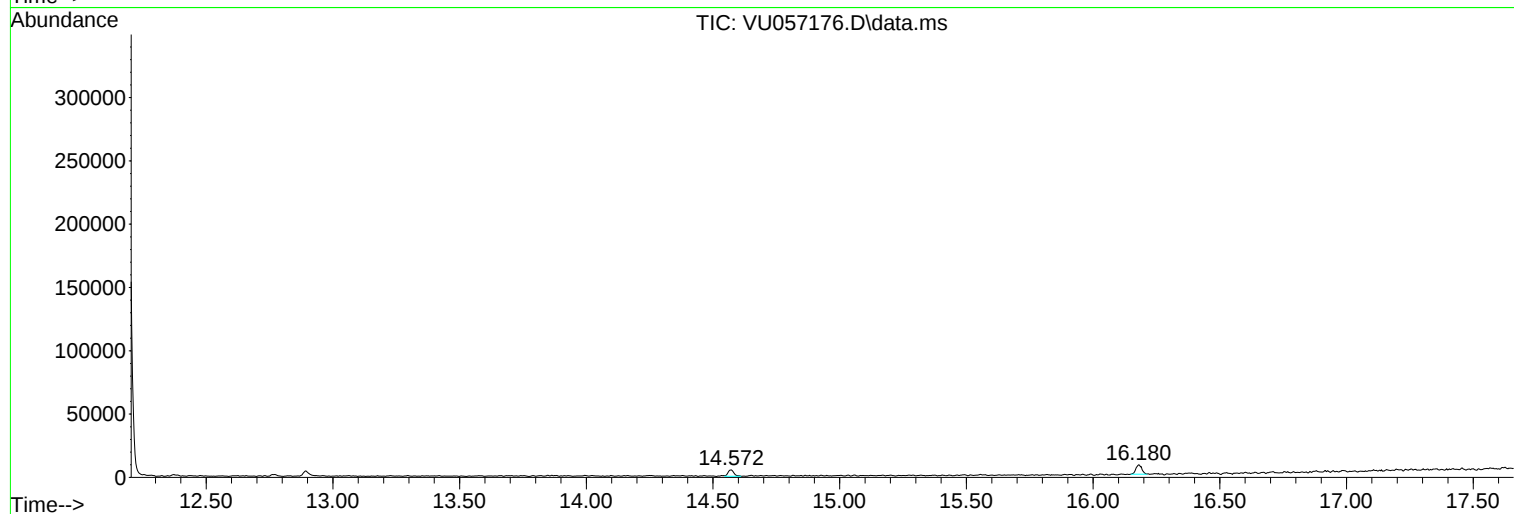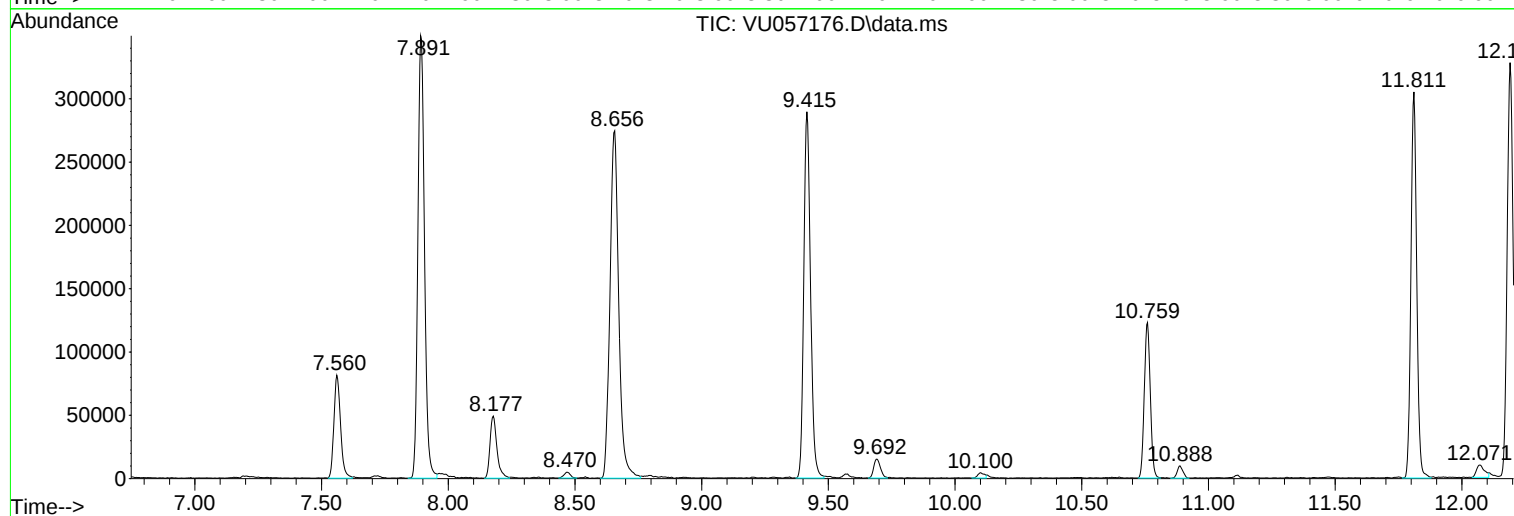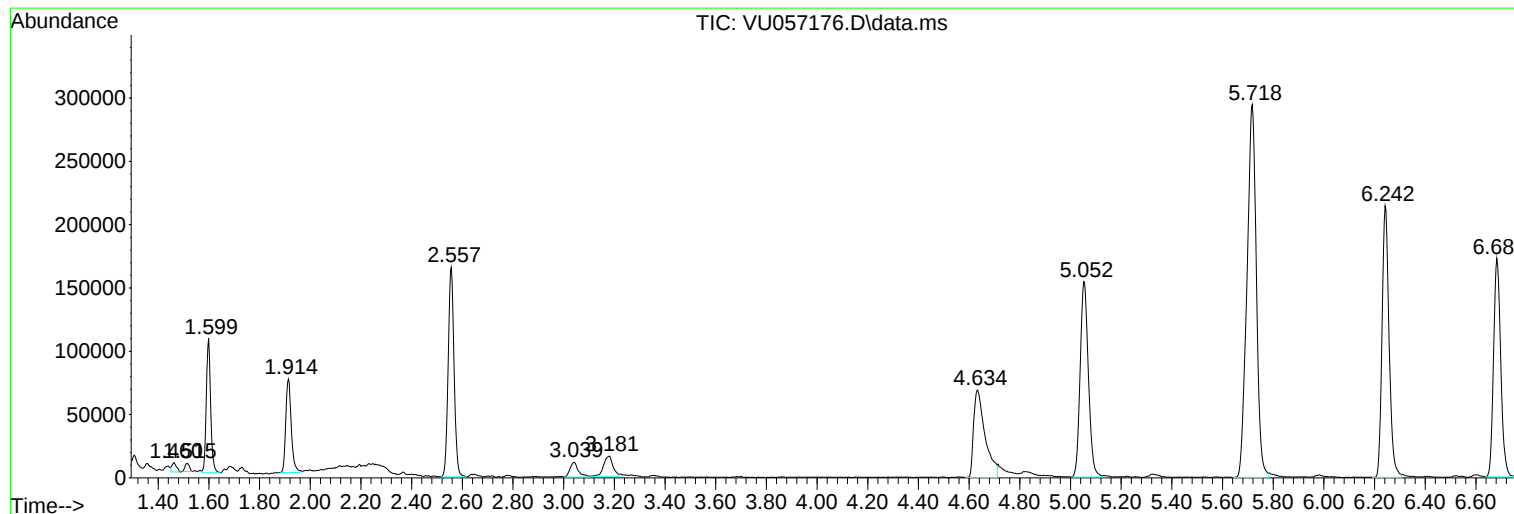

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122123\
Data File : VU057176.D
Acq On : 22 Dec 2023 08:31
Operator : MD/SY
Sample : 05912-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH3P5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122123\
Data File : VU057176.D
Acq On : 22 Dec 2023 08:31
Operator : MD/SY
Sample : 05912-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 53 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH3P5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc