


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122123\
Data File : VU057126.D
Acq On : 21 Dec 2023 08:44
Operator : MD/SY
Sample : BFB099
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB099

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Dec 22 01:33:10 2023

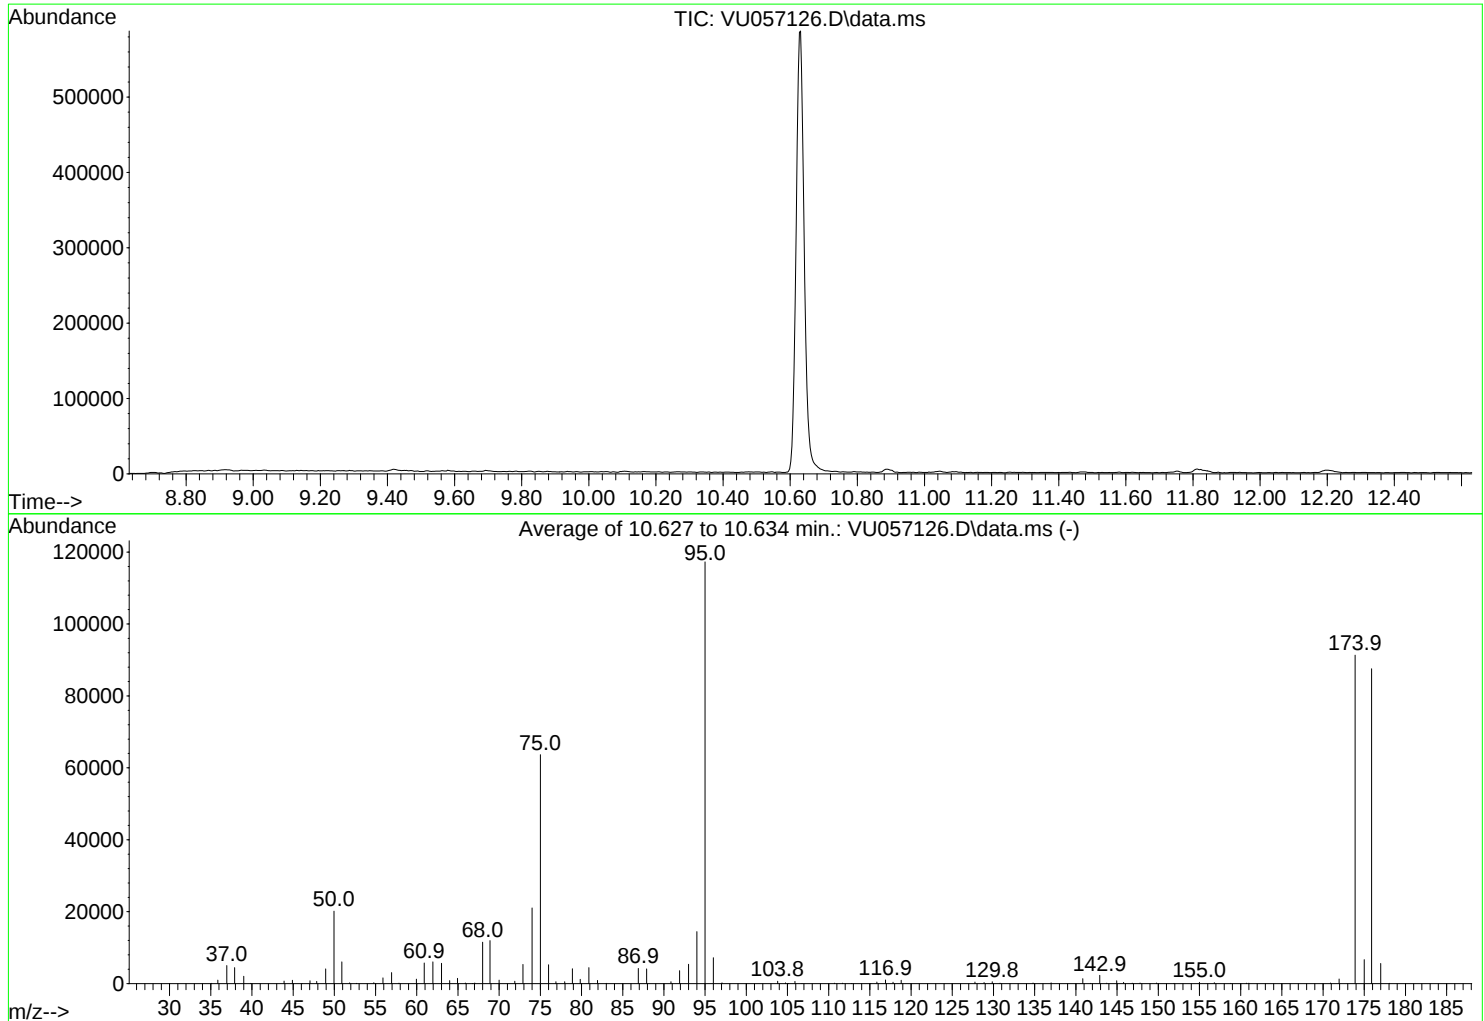

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	20141	PASS
75	95	30	80	54.3	63683	PASS
95	95	100	100	100.0	117280	PASS
96	95	5	9	6.2	7227	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	77.9	91328	PASS
175	174	5	9	7.3	6672	PASS
176	174	95	101	95.9	87557	PASS
177	176	5	9	6.4	5622	PASS

m/z	Abundance
35.90	1104.0
37.80	402.0
39.80	262.0
43.90	242.0

Instrument :
MSVOA_U
ClientSampleId :
BFB099

m/z	Abundance
35.10	249.0
35.80	2058.0
37.00	5204.0
37.90	4933.0
39.00	2108.0
39.90	349.0
43.90	920.0
44.90	1135.0
46.10	138.0
47.10	952.0
47.80	696.0
48.90	4422.0
50.00	21096.0
50.90	6355.0
51.90	167.0
52.70	179.0
54.80	247.0
55.90	1512.0
56.90	3177.0
57.90	115.0
59.90	1289.0
60.90	6063.0
61.90	6382.0
63.00	5723.0
64.00	760.0
65.00	1594.0
65.90	208.0
66.80	186.0
68.00	11913.0
68.90	12085.0
70.00	1152.0
71.90	685.0
72.90	5656.0
74.00	21552.0
75.00	65664.0
76.00	5495.0
77.00	568.0
78.00	668.0
78.90	4490.0
79.90	1192.0
80.90	4662.0
82.00	976.0
86.90	4325.0
87.90	4378.0
90.80	558.0
91.90	3811.0
93.00	5529.0
94.00	14860.0
95.00	119232.0
96.00	7623.0
97.00	199.0
103.80	661.0
104.70	169.0
105.10	174.0
105.90	623.0
106.80	104.0
110.70	138.0
111.70	116.0
115.80	427.0
116.90	1047.0
117.80	399.0
118.80	1012.0
127.80	432.0
128.80	287.0
129.90	516.0
130.80	203.0
134.90	204.0
137.00	280.0
140.90	1429.0
141.80	151.0
142.90	2526.0
143.80	152.0
144.90	823.0
145.80	368.0
146.90	120.0
147.80	189.0
149.80	108.0
151.90	124.0
155.00	367.0
156.80	223.0
158.80	137.0
161.00	276.0
170.90	184.0
172.00	1338.0
173.90	93112.0
175.00	6618.0
175.90	89800.0
177.00	5531.0
178.00	112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB099

m/z	Abundance
35.80	2131.0
36.90	5203.0
37.90	5044.0
39.00	2168.0
40.00	350.0
43.90	942.0
44.90	994.0
47.10	793.0
47.90	656.0
48.90	4172.0
50.00	20744.0
50.90	6262.0
51.90	197.0
52.70	130.0
54.80	294.0
55.90	1613.0
57.00	3103.0
57.90	123.0
59.90	1308.0
60.90	5795.0
61.90	6336.0
63.00	5743.0
64.00	847.0
64.90	1545.0
65.90	156.0
67.10	254.0
68.00	11919.0
68.90	12297.0
70.00	997.0
71.90	706.0
72.90	5497.0
74.00	21776.0
75.00	65808.0
76.00	5292.0
76.90	490.0
77.90	504.0
78.90	4264.0
79.90	1252.0
80.90	4618.0
82.00	947.0
83.00	132.0
86.90	4271.0
87.90	4194.0
90.80	530.0
91.90	3606.0
93.00	5577.0
94.00	14790.0
95.00	120752.0
96.00	7313.0
97.10	232.0
103.80	717.0
104.80	262.0
105.90	685.0
106.70	108.0
110.70	158.0
111.70	146.0
115.80	436.0
116.90	1040.0
117.80	385.0
118.80	941.0
127.70	496.0
128.90	280.0
129.90	549.0
130.80	169.0
134.80	180.0
137.00	232.0
140.90	1407.0
141.80	120.0
142.90	2361.0
143.70	124.0
144.90	825.0
145.80	409.0
146.90	156.0
147.80	160.0
149.80	167.0
151.90	112.0
155.00	385.0
156.80	271.0
158.80	112.0
160.70	191.0
161.00	167.0
170.90	177.0
171.90	1330.0
173.90	94528.0
175.00	6881.0
175.90	90496.0
177.00	5747.0
178.10	114.0

Instrument :
MSVOA_U
ClientSampleId :
BFB099

m/z	Abundance
35.90	2007.0
36.90	4694.0
38.00	4519.0
39.00	1884.0
39.90	366.0
43.90	1012.0
44.90	711.0
47.00	595.0
47.90	568.0
49.00	3742.0
49.90	18584.0
50.90	5551.0
51.80	257.0
54.80	314.0
55.90	1631.0
57.00	2914.0
57.80	134.0
60.00	1180.0
60.90	5308.0
62.00	5488.0
63.00	5453.0
64.00	910.0
65.00	1299.0
65.90	120.0
67.00	320.0
68.00	10690.0
68.90	11475.0
70.00	786.0
71.90	647.0
72.90	4831.0
74.00	19800.0
75.00	59576.0
76.00	4966.0
76.80	523.0
77.90	407.0
78.90	3617.0
79.80	1204.0
80.90	4145.0
81.90	803.0
83.00	192.0
86.90	4118.0
87.90	3708.0
90.90	486.0
91.90	3464.0
93.00	5046.0
94.00	13682.0
95.00	111856.0
96.00	6746.0
97.10	275.0
103.80	641.0
104.80	307.0
105.90	545.0
110.70	124.0
111.70	145.0
112.80	117.0
115.10	108.0
115.90	434.0
116.90	966.0
117.80	391.0
118.80	811.0
127.70	466.0
128.90	316.0
129.80	548.0
130.80	105.0
134.70	207.0
137.00	156.0
140.80	1317.0
142.90	2022.0
143.80	101.0
145.00	722.0
145.80	354.0
146.80	162.0
147.80	183.0
149.80	224.0
155.00	360.0
156.80	273.0
160.70	176.0
170.90	181.0
172.00	1186.0
173.90	86344.0
175.00	6516.0
175.90	82376.0
177.00	5588.0

Instrument :
MSVOA_U
ClientSampleId :
BFB099