


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU122218\
Data File : VU028908.D
Acq On : 22 Dec 2018 09:57
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U120618W.M
Title : SW846 8260
Last Update : Fri Dec 07 00:39:42 2018

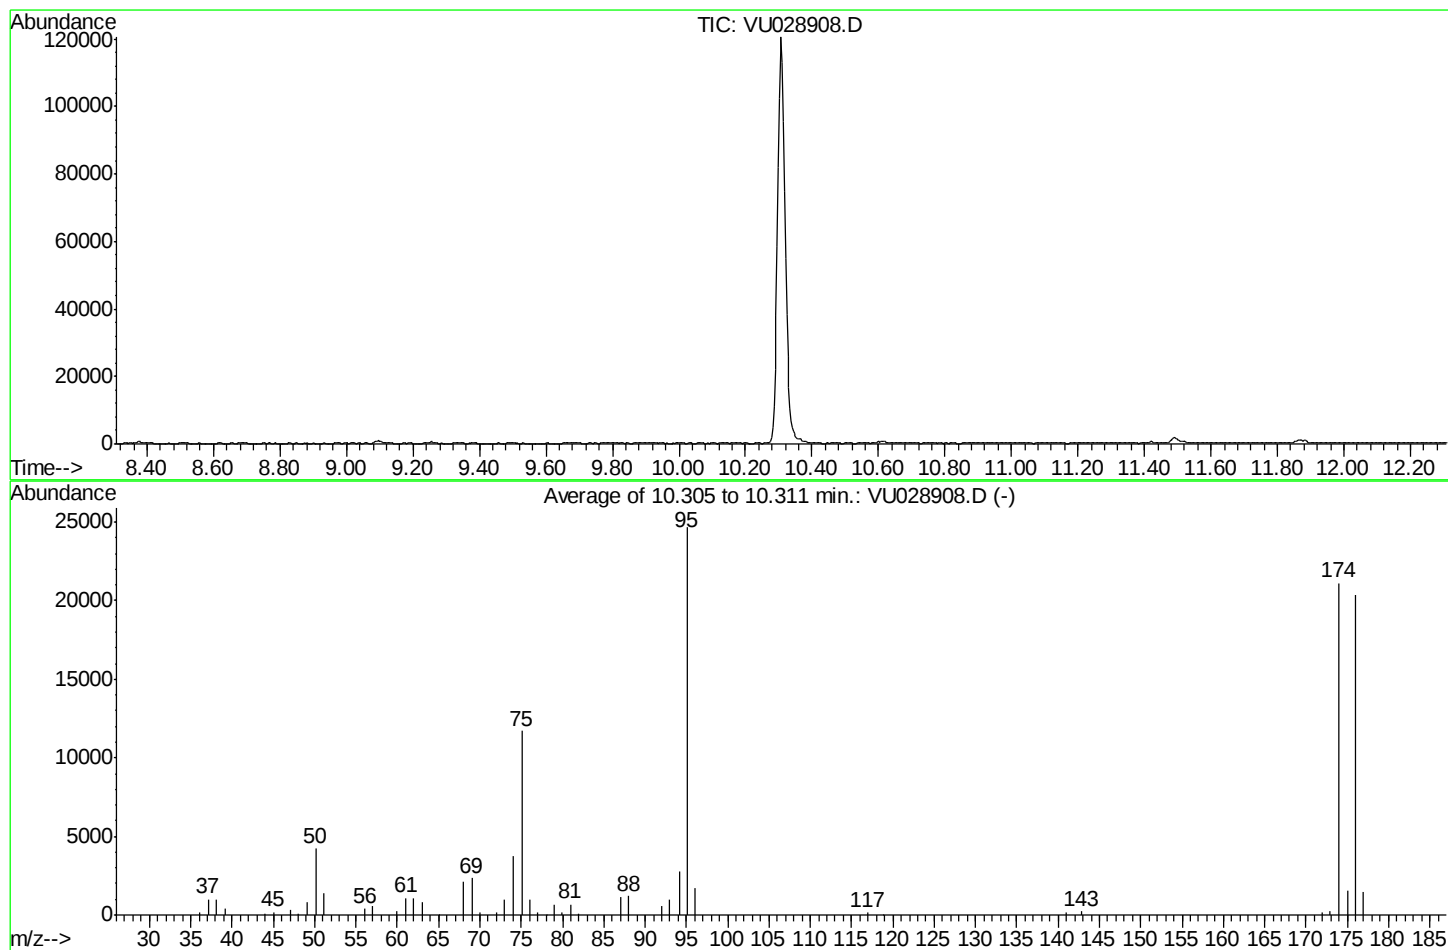

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	4198	PASS
75	95	30	60	47.5	11727	PASS
95	95	100	100	100.0	24669	PASS
96	95	5	9	6.9	1694	PASS
173	174	0.00	2	1.1	230	PASS
174	95	50	100	85.7	21130	PASS
175	174	5	9	7.3	1533	PASS
176	174	95	101	96.4	20360	PASS
177	176	5	9	7.0	1432	PASS