


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU122220\
Data File : VU041764.D
Acq On : 23 Dec 2020 00:24
Operator : SY/MD
Sample : L5161-21
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB246

Manual Integrations
APPROVED

SAM
12/23/2020 5:49:39 PM

Quant Time: Dec 23 07:58:31 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Dec 23 05:08:09 2020
Response via : Initial Calibration

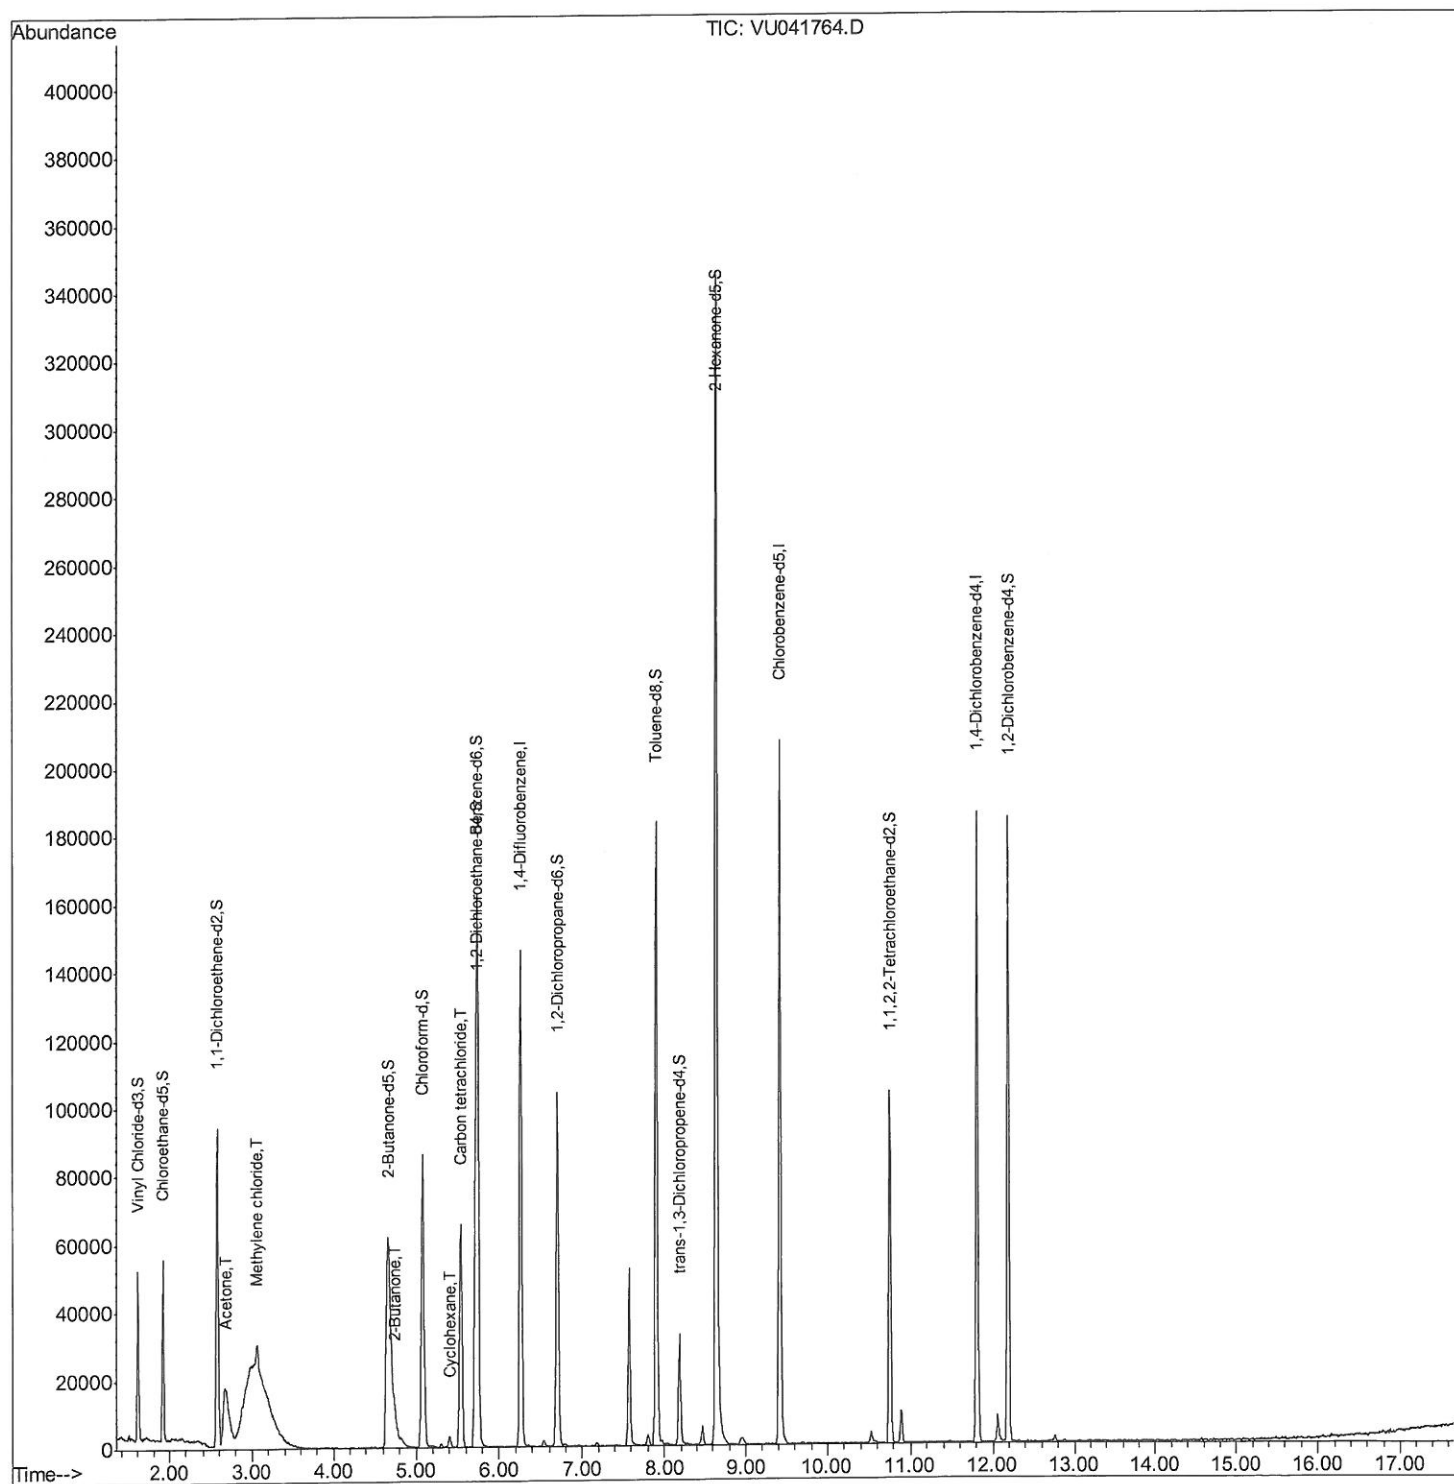

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU122220\
 Data File : VU041764.D
 Acq On : 23 Dec 2020 00:24
 Operator : SY/MD
 Sample : L5161-21
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB246

Manual Integrations
 APPROVED

SAM
 12/23/2020 5:49:39 PM

Quant Time: Dec 23 05:11:40 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Dec 23 05:08:09 2020
 Response via : Initial Calibration

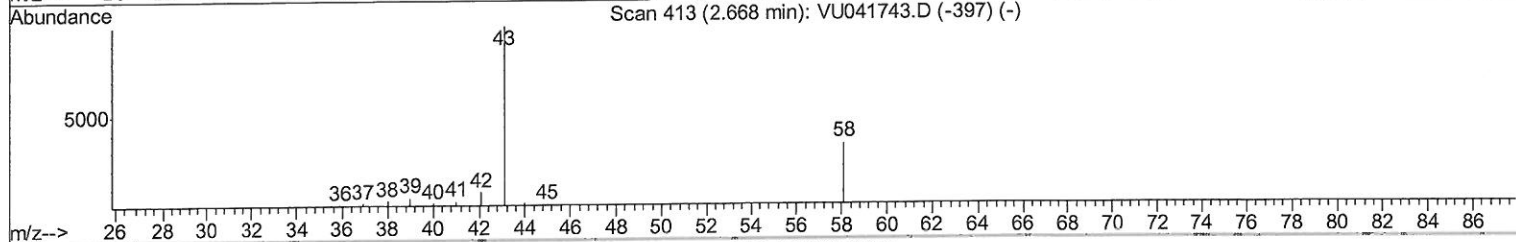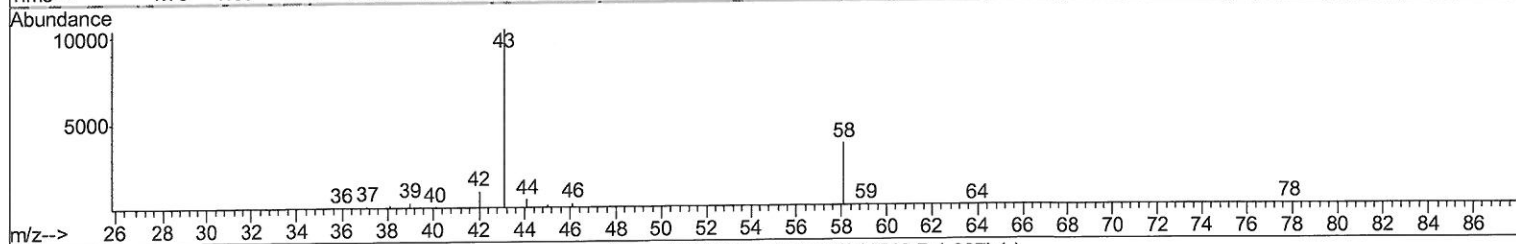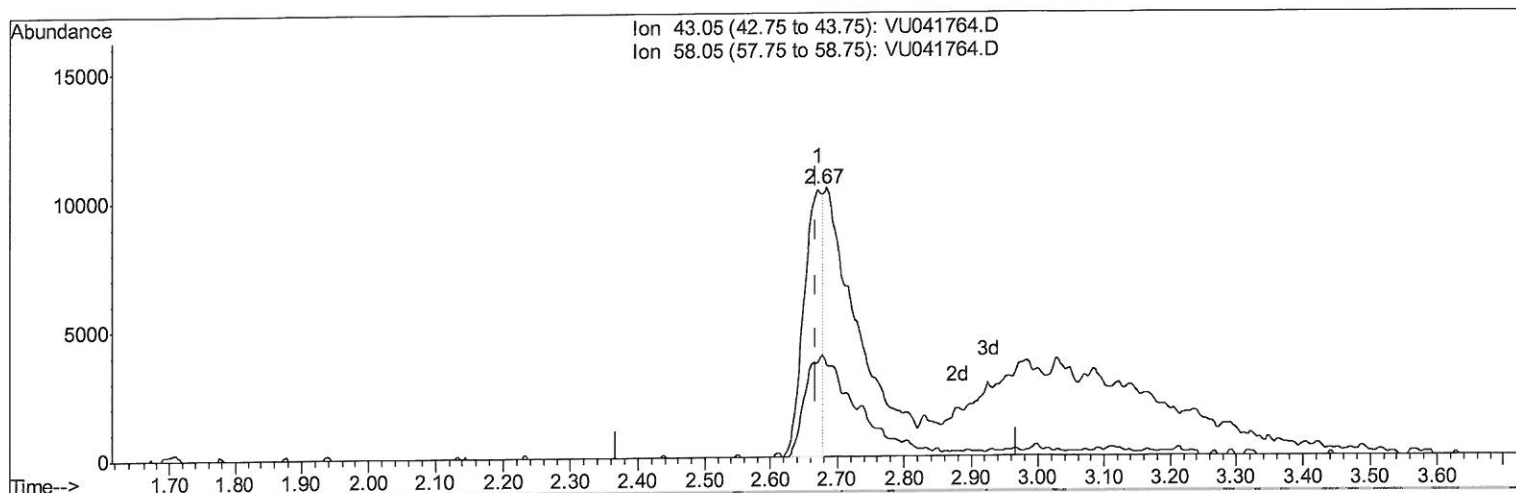

(13) Acetone (T)

2.671min (+0.003) 11.32ug/L

response 20133

Ion	Exp%	Act%
43.05	100	100
58.05	36.60	79.49#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU122220\
Data File : VU041764.D
Acq On : 23 Dec 2020 00:24
Operator : SY/MD
Sample : L5161-21
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB246

Manual Integrations
APPROVED

SAM
12/23/2020 5:49:39 PM

Quant Time: Dec 23 05:11:40 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Dec 23 05:08:09 2020
Response via : Initial Calibration

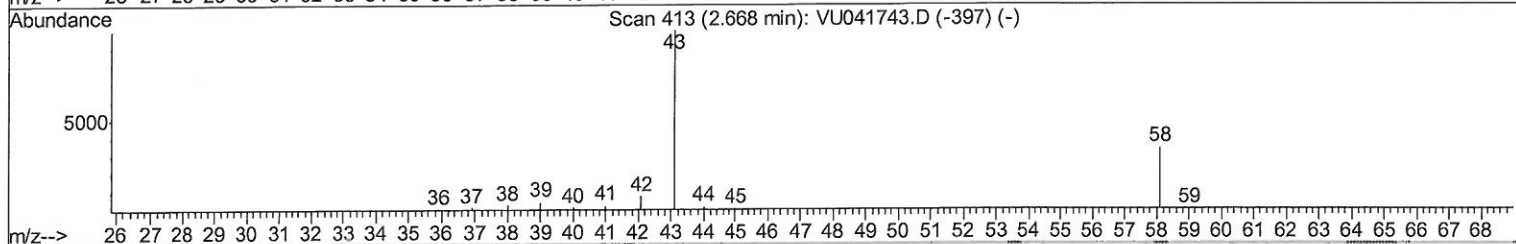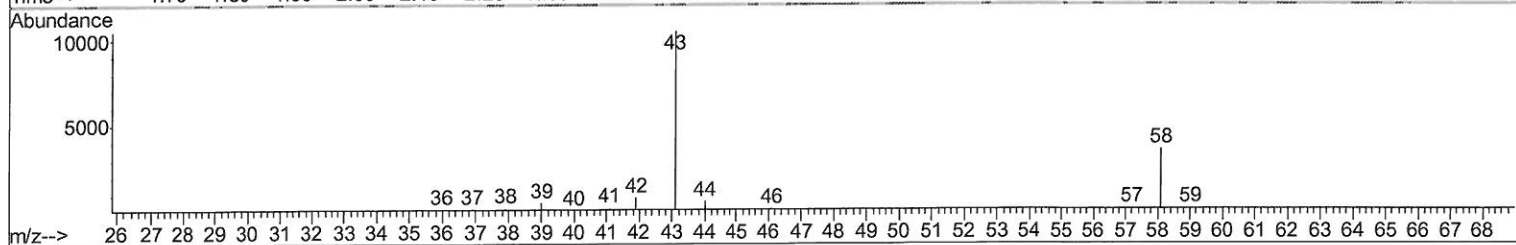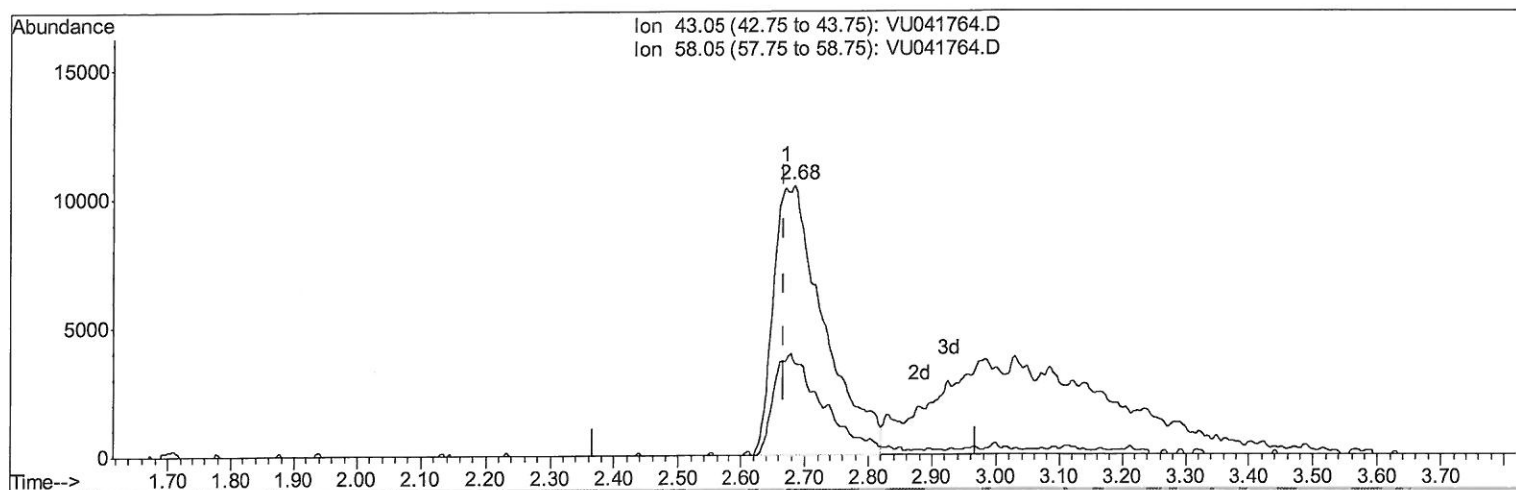

TIC: VU041764.D

(13) Acetone (T)

2.684min (+0.016) 32.32ug/L m

response 57485

Ion	Exp%	Act%
43.05	100	100
58.05	36.60	27.84
0.00	0.00	0.00
0.00	0.00	0.00

SY/MD
12/23/20

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU122220\
Data File : VU041764.D
Acq On : 23 Dec 2020 00:24
Operator : SY/MD
Sample : L5161-21
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB246

Manual Integrations
APPROVED

SAM
12/23/2020 5:49:39 PM

Quant Time: Dec 23 07:55:47 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Dec 23 05:08:09 2020
Response via : Initial Calibration

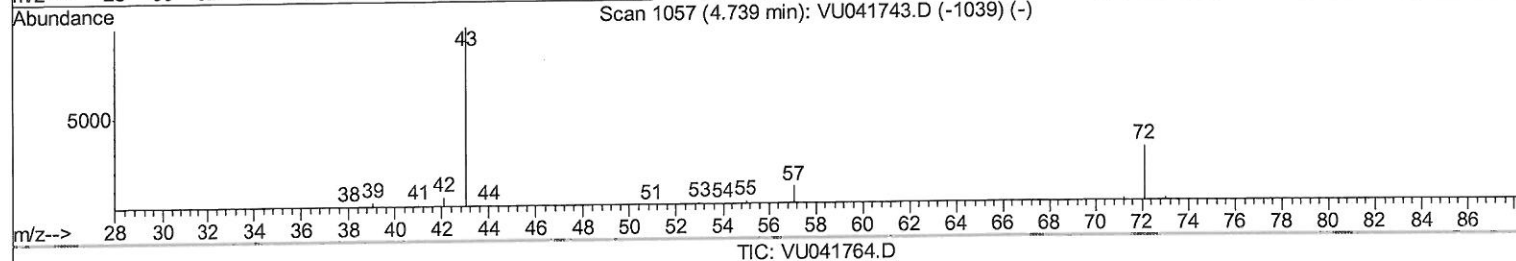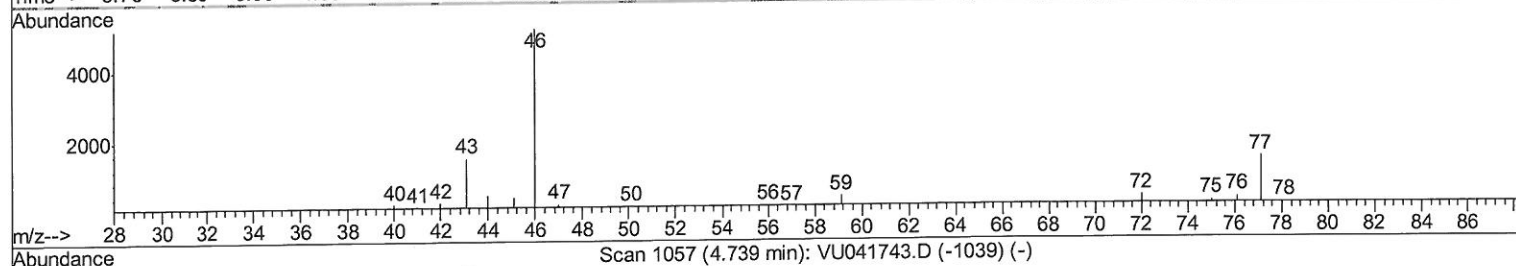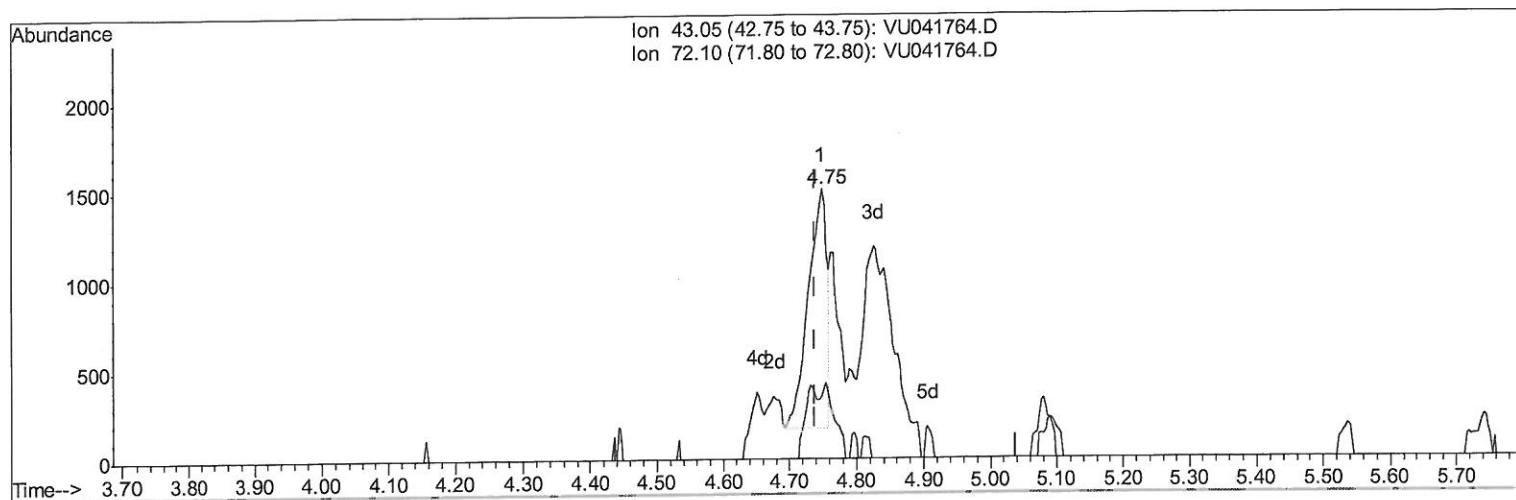

(21) 2-Butanone (T)

4.748min (+0.010) 0.88ug/L

response 2554

Ion	Exp%	Act%
43.05	100	100
72.10	29.30	22.16
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU122220\
Data File : VU041764.D
Acq On : 23 Dec 2020 00:24
Operator : SY/MD
Sample : L5161-21
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB246

Manual Integrations
APPROVED

SAM
12/23/2020 5:49:39 PM

Quant Time: Dec 23 07:55:47 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Dec 23 05:08:09 2020
Response via : Initial Calibration

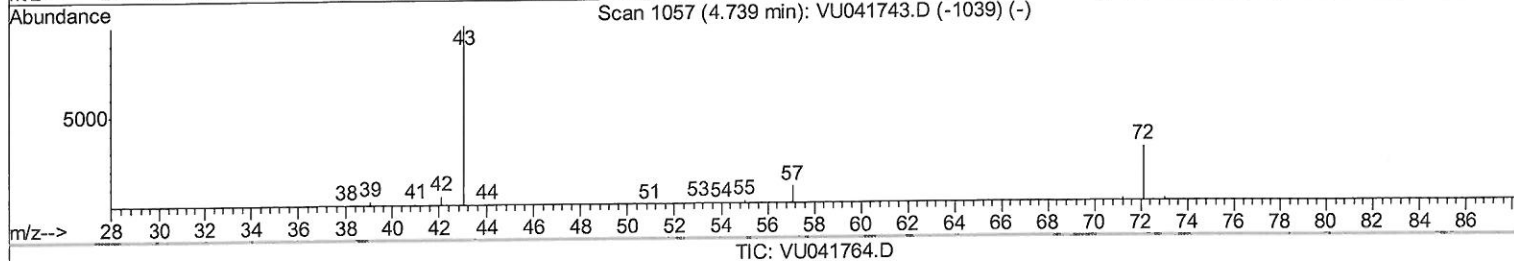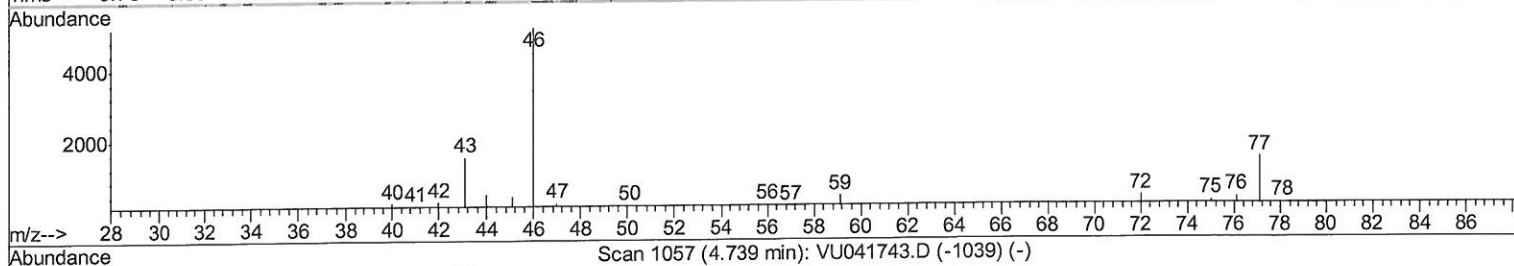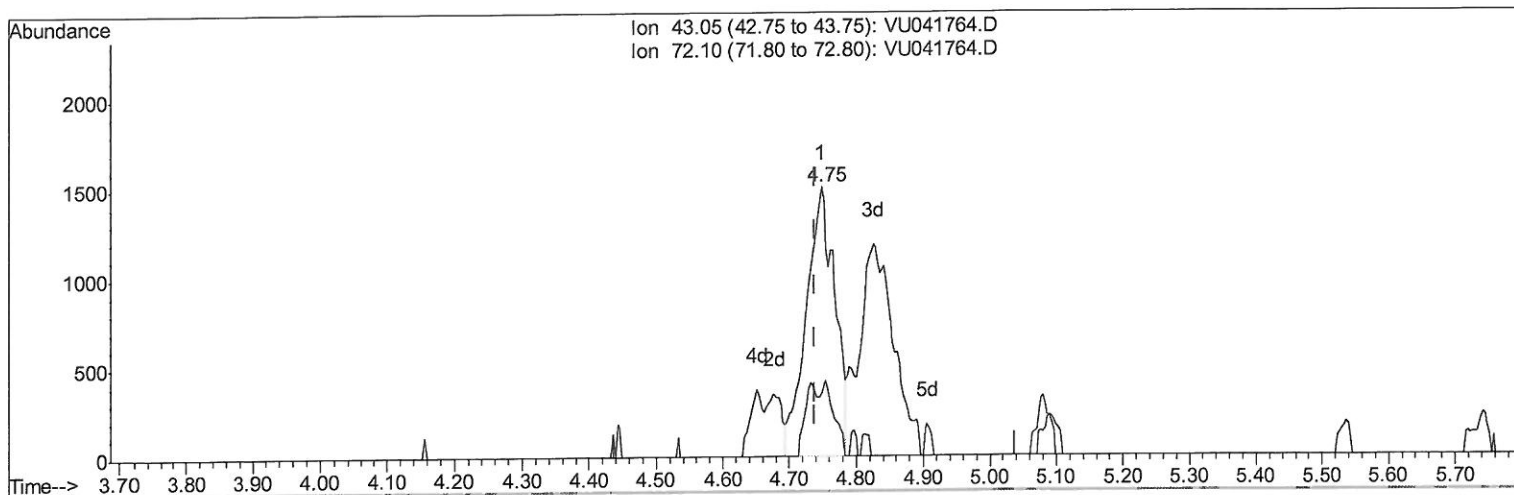

(21) 2-Butanone (T)

4.748min (+0.010) 1.54ug/L m

response 4452

Ion	Exp%	Act%
43.05	100	100
72.10	29.30	12.71#
0.00	0.00	0.00
0.00	0.00	0.00

7 mg
12/23/20

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU122220\
 Data File : VU041764.D
 Acq On : 23 Dec 2020 00:24
 Operator : SY/MD
 Sample : L5161-21
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB246

Manual Integrations
 APPROVED

SAM
 12/23/2020 5:49:39 PM

Quant Time: Dec 23 07:58:31 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Dec 23 05:08:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Difluorobenzene	6.26	114	124507	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	119731	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	51238	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	33438	3.44	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.80%
7) Chloroethane-d5	1.92	69	37817	5.02	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.40%
11) 1,1-Dichloroethene-d2	2.58	63	56815	3.17	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.40%
20) 2-Butanone-d5	4.66	46	159604	57.08	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.16%
24) Chloroform-d	5.08	84	81664	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
26) 1,2-Dichloroethane-d4	5.72	65	47422	5.01	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.20%
32) Benzene-d6	5.74	84	156163	4.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.20%
36) 1,2-Dichloropropane-d6	6.70	67	51741	4.81	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.20%
41) Toluene-d8	7.90	98	125497	4.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.20%
43) trans-1,3-Dichloropropene-	8.19	79	19494	4.03	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.60%
46) 2-Hexanone-d5	8.64	63	136516	51.67	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.34%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	52579	5.38	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	107.60%
64) 1,2-Dichlorobenzene-d4	12.19	152	50181	5.51	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.20%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
13) Acetone	2.68	43	57485m	32.322	ug/L	
16) Methylene chloride	3.06	84	3622	0.359	ug/L	81
21) 2-Butanone	4.75	43	4452m	1.537	ug/L	
30) Cyclohexane	5.40	56	1615	0.105	ug/L #	43
31) Carbon tetrachloride	5.54	117	45169	3.799	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed