

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U122220\
 Data File : VU041741.D
 Acq On : 22 Dec 2020 15:02
 Operator : SY/MD
 Sample : L5162-09DL 20X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB255DL

Quant Time: Dec 23 05:02:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Dec 23 04:05:15 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	131140	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	127032	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	56785	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	34840	3.40	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.00%
7) Chloroethane-d5	1.92	69	41076	5.18	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	103.60%
11) 1,1-Dichloroethene-d2	2.58	63	58994	3.12	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.40%
20) 2-Butanone-d5	4.67	46	170874	58.02	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	116.04%
24) Chloroform-d	5.08	84	87598	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.80%
26) 1,2-Dichloroethane-d4	5.72	65	50432	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.20%
32) Benzene-d6	5.74	84	167527	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.20%
36) 1,2-Dichloropropane-d6	6.70	67	55943	4.91	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.20%
41) Toluene-d8	7.90	98	137557	4.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	83.80%
43) trans-1,3-Dichloropropene-	8.18	79	23110	4.51	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	90.20%
46) 2-Hexanone-d5	8.64	63	146625	52.30	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	104.60%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	54231	5.23	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.60%
64) 1,2-Dichlorobenzene-d4	12.19	152	54615	5.41	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.20%


Target Compounds					Ovalue
31) Carbon tetrachloride	5.54	117	83082	6.586 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU122220\
Data File : VU041741.D
Acq On : 22 Dec 2020 15:02
Operator : SY/MD
Sample : L5162-09DL 20X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB255DL

Quant Time: Dec 23 05:02:49 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Dec 23 04:05:15 2020
Response via : Initial Calibration

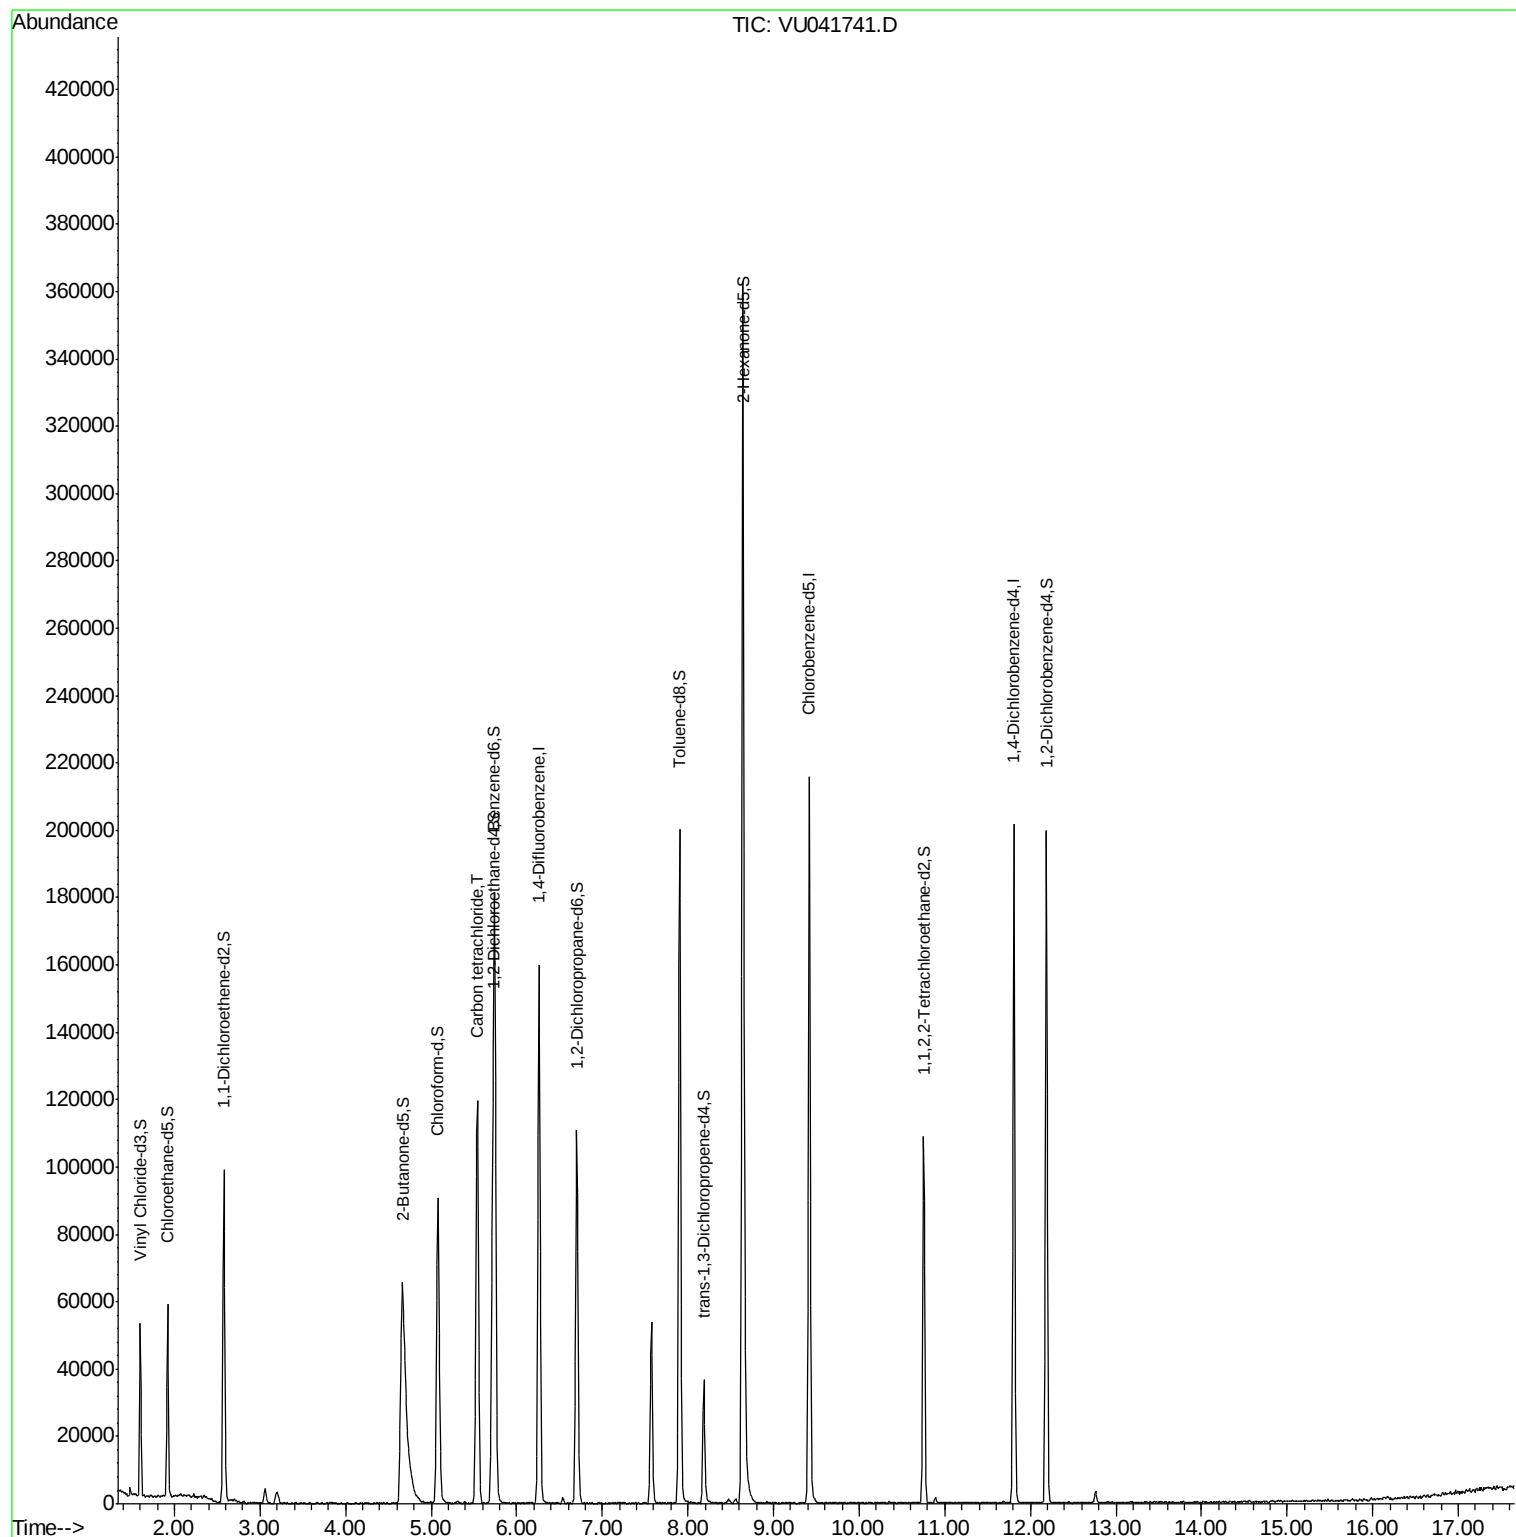

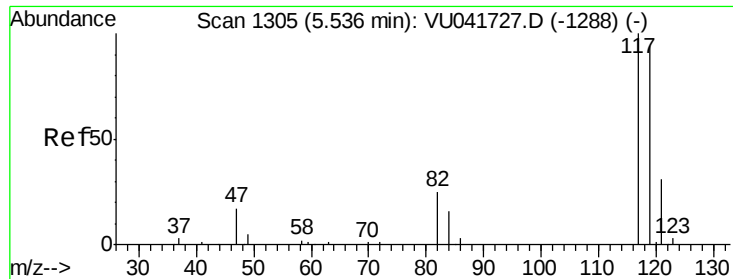

#31

Carbon tetrachloride

Concen: 6.586 ug/L

RT: 5.54 min Scan# 1306

Delta R.T. 0.00 min

Lab File: VU041741.D

Acq: 22 Dec 2020 15:02

Instrument :

MSVOA_U

ClientSampleId :

GB255DL

Tot Ion:117 Resp: 83082

Ion Ratio Lower Upper

117 100

119 96.4 76.2 114.2

