

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U122220\
 Data File : VU041765.D
 Acq On : 23 Dec 2020 00:48
 Operator : SY/MD
 Sample : L5161-11DL 2X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB236DL

Quant Time: Dec 23 07:06:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Dec 23 05:08:09 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	130141	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	124565	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	55347	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	35153	3.46	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	69.20%
7) Chloroethane-d5	1.92	69	39401	5.00	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.00%
11) 1,1-Dichloroethene-d2	2.58	63	56333	3.01	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.20%
20) 2-Butanone-d5	4.67	46	163087	55.80	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.60%
24) Chloroform-d	5.08	84	85271	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.80%
26) 1,2-Dichloroethane-d4	5.72	65	51328	5.19	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.80%
32) Benzene-d6	5.74	84	162173	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.00%
36) 1,2-Dichloropropane-d6	6.70	67	53615	4.79	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.80%
41) Toluene-d8	7.91	98	132232	4.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.20%
43) trans-1,3-Dichloropropene-	8.19	79	21030	4.18	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.60%
46) 2-Hexanone-d5	8.64	63	145213	52.83	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	105.66%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	56570	5.57	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	111.40%
64) 1,2-Dichlorobenzene-d4	12.19	152	51508	5.23	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.60%


Target Compounds					Ovalue
31) Carbon tetrachloride	5.54	117	127008	10.268 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU122220\
Data File : VU041765.D
Acq On : 23 Dec 2020 00:48
Operator : SY/MD
Sample : L5161-11DL 2X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB236DL

Quant Time: Dec 23 07:06:49 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Dec 23 05:08:09 2020
Response via : Initial Calibration

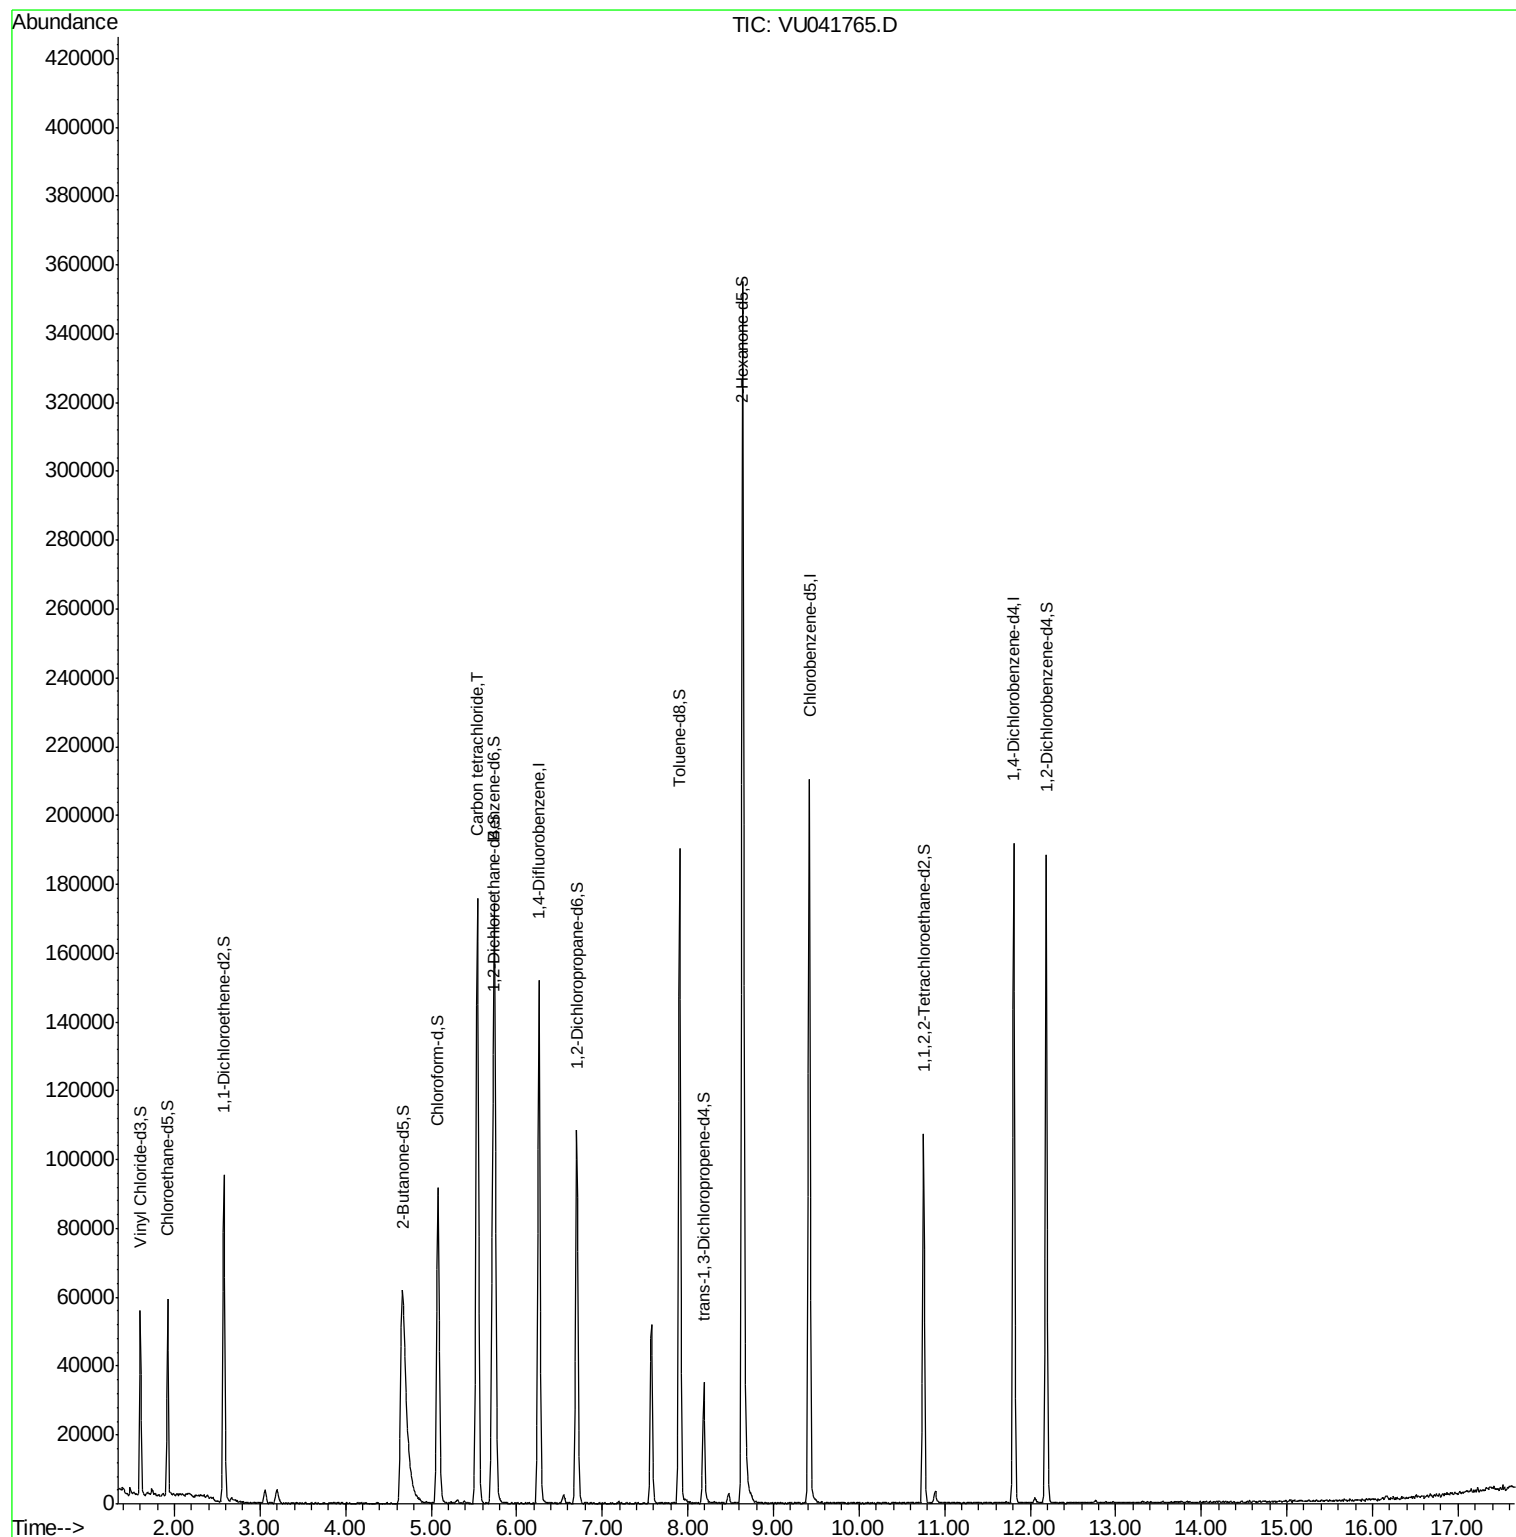

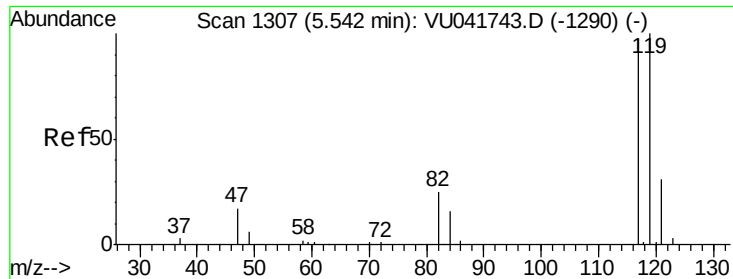

#31

Carbon tetrachloride

Concen: 10.268 ug/L

RT: 5.54 min Scan# 1306

Delta R.T. -0.00 min

Lab File: VU041765.D

Acq: 23 Dec 2020 00:48

Instrument :

MSVOA_U

ClientSampleId :


GB236DL

Tot Ion:117 Resp: 127008

Ion Ratio Lower Upper

117 100

119 95.8 76.2 114.2

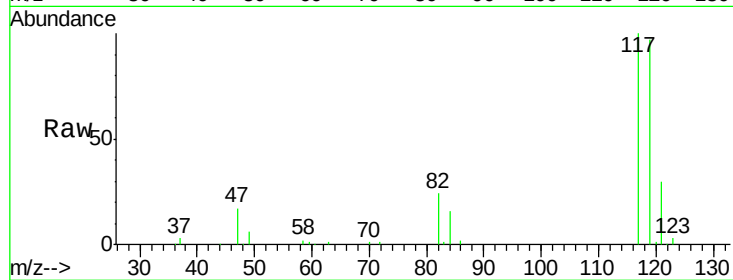

Abundance Ion 116.90 (116.60 to 117.60): V

Ion 118.90 (118.60 to 119.60): V

