


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU122220\
Data File : VU041726.D
Acq On : 22 Dec 2020 08:43
Operator : SY/MD
Sample : BFB28
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB28

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Dec 23 05:08:09 2020

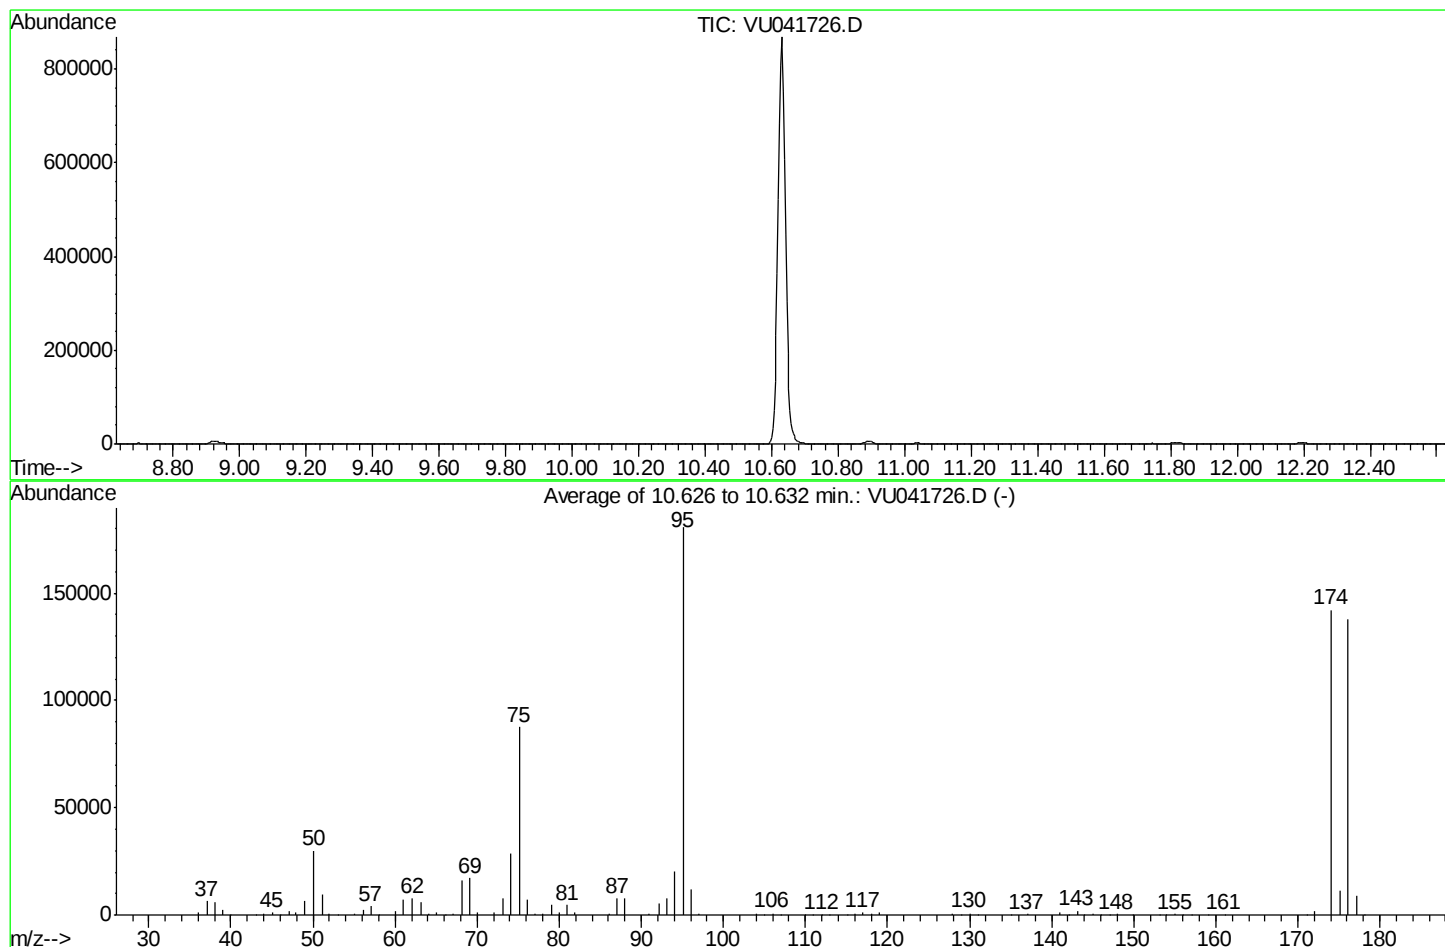

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2874

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	30010	PASS
75	95	30	80	48.4	87533	PASS
95	95	100	100	100.0	180714	PASS
96	95	5	9	6.8	12241	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.8	142314	PASS
175	174	5	9	7.9	11188	PASS
176	174	95	101	96.9	137970	PASS
177	176	5	9	6.6	9089	PASS

m/z	Abundance
36.10	1346.0
37.10	6324.0
38.00	5943.0
39.00	2402.0
39.90	182.0
44.00	1156.0
45.10	997.0
45.90	190.0
47.00	1756.0
48.00	1100.0
49.00	6287.0
50.10	29528.0
51.10	9402.0
52.00	392.0
53.00	167.0
55.10	305.0
56.10	2208.0
57.10	3739.0
58.00	254.0
60.10	1662.0
61.10	7114.0
62.10	7390.0
63.10	5992.0
64.10	926.0
65.10	1293.0
66.10	113.0
67.10	374.0
68.10	15724.0
69.10	16856.0
70.10	1340.0
72.10	926.0
73.10	7978.0
74.10	28528.0
75.10	85320.0
76.10	6971.0
77.00	760.0
77.90	714.0
79.00	4555.0
80.00	1290.0
81.00	4589.0
82.00	1134.0
86.10	302.0
87.00	7662.0
88.00	7524.0
91.00	517.0
92.10	5220.0
93.10	7547.0
94.10	19848.0
95.10	173248.0
96.10	12023.0
97.00	315.0
104.00	629.0
105.00	300.0
106.00	669.0
106.90	176.0
111.00	135.0
112.00	169.0
112.90	122.0
115.10	275.0
116.00	567.0
117.00	1187.0
118.00	578.0
119.00	982.0
127.90	531.0
129.00	283.0
130.00	615.0
131.00	165.0
135.00	308.0
137.00	301.0
141.00	1206.0
142.10	131.0
143.10	1918.0
144.00	135.0
145.10	415.0
146.00	308.0
148.00	332.0
149.90	107.0
153.20	109.0
154.00	229.0
155.10	283.0
157.00	232.0
159.10	268.0
161.00	169.0
171.10	202.0
172.10	1707.0
174.10	134336.0
175.10	11017.0
176.10	129624.0
177.10	8653.0
178.10	275.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28

m/z	Abundance
36.10	1367.0
37.10	6541.0
38.00	6045.0
39.10	2564.0
40.00	180.0
44.00	1144.0
45.00	1098.0
45.90	213.0
47.00	1923.0
47.90	1120.0
49.10	6632.0
50.10	31208.0
51.10	9871.0
52.00	384.0
53.00	190.0
55.00	362.0
56.10	2471.0
57.10	4105.0
58.00	301.0
60.10	1694.0
61.00	7384.0
62.10	7882.0
63.10	6368.0
64.10	930.0
65.10	1359.0
66.10	163.0
67.10	418.0
68.10	16736.0
69.10	17952.0
70.00	1416.0
72.10	1111.0
73.10	8089.0
74.10	29680.0
75.10	90328.0
76.10	7527.0
77.10	832.0
77.90	702.0
79.00	4644.0
80.00	1464.0
81.00	4737.0
81.90	1234.0
86.10	386.0
87.00	8024.0
88.00	7953.0
91.00	563.0
92.10	5456.0
93.10	7982.0
94.10	21152.0
95.10	186304.0
96.10	12511.0
97.10	339.0
104.00	668.0
105.00	235.0
106.00	707.0
107.00	219.0
109.90	108.0
110.90	161.0
112.00	217.0
112.90	104.0
115.10	210.0
116.00	640.0
117.00	1195.0
118.00	632.0
119.00	1069.0
128.00	569.0
129.00	301.0
130.00	703.0
131.00	222.0
135.00	317.0
137.00	351.0
141.00	1372.0
142.10	160.0
143.10	1935.0
144.00	145.0
145.10	502.0
146.00	289.0
148.00	377.0
149.90	133.0
153.10	130.0
154.00	236.0
155.10	386.0
157.00	289.0
159.10	268.0
161.10	173.0
171.10	159.0
172.10	1745.0
174.10	146688.0
175.10	11535.0
176.10	142592.0
177.10	9393.0
178.10	248.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28

m/z	Abundance
36.00	1214.0
37.10	6185.0
38.00	5650.0
39.10	2601.0
40.00	184.0
43.00	109.0
44.00	996.0
45.00	1170.0
46.00	191.0
47.10	1847.0
48.00	1008.0
49.10	6374.0
50.10	29296.0
51.10	9338.0
51.90	372.0
52.90	200.0
55.00	391.0
56.10	2407.0
57.00	4032.0
58.10	266.0
60.10	1494.0
61.00	7358.0
62.10	7740.0
63.10	6166.0
64.10	839.0
65.10	1186.0
66.20	222.0
67.00	435.0
68.10	16310.0
69.10	17024.0
70.00	1278.0
72.10	1212.0
73.10	7202.0
74.10	27712.0
75.10	86952.0
76.10	7458.0
77.00	893.0
78.00	663.0
79.00	4374.0
80.00	1506.0
81.00	4545.0
81.90	1185.0
86.10	401.0
87.10	7513.0
88.00	7632.0
90.90	542.0
92.10	5021.0
93.10	7556.0
94.10	20256.0
95.10	182592.0
96.10	12191.0
97.10	328.0
104.00	634.0
104.90	164.0
106.00	637.0
107.00	233.0
109.90	117.0
110.90	135.0
112.00	151.0
115.10	148.0
116.00	549.0
117.00	1214.0
118.00	589.0
119.10	1046.0
128.00	574.0
129.00	300.0
130.00	654.0
131.00	258.0
135.00	273.0
137.10	363.0
141.00	1509.0
142.00	193.0
143.10	1820.0
143.90	131.0
145.10	489.0
146.10	225.0
147.00	124.0
147.90	397.0
149.90	137.0
153.00	117.0
154.00	165.0
155.10	412.0
156.00	100.0
157.10	323.0
159.10	258.0
161.10	164.0
171.00	117.0
172.10	1612.0
174.10	145920.0
175.10	11012.0
176.10	141696.0
177.10	9221.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28

178.10

196.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28

Scan 2874 (10.581 min): VU041726.D
BFB28

m/z	Abundance
39.90	141.0
44.00	221.0

Instrument :
MSVOA_U
ClientSampleId :
BFB28