


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122221\
Data File : VU046548.D
Acq On : 22 Dec 2021 10:40
Operator : SY/MD
Sample : BFB034
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB034

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Dec 30 04:21:35 2021

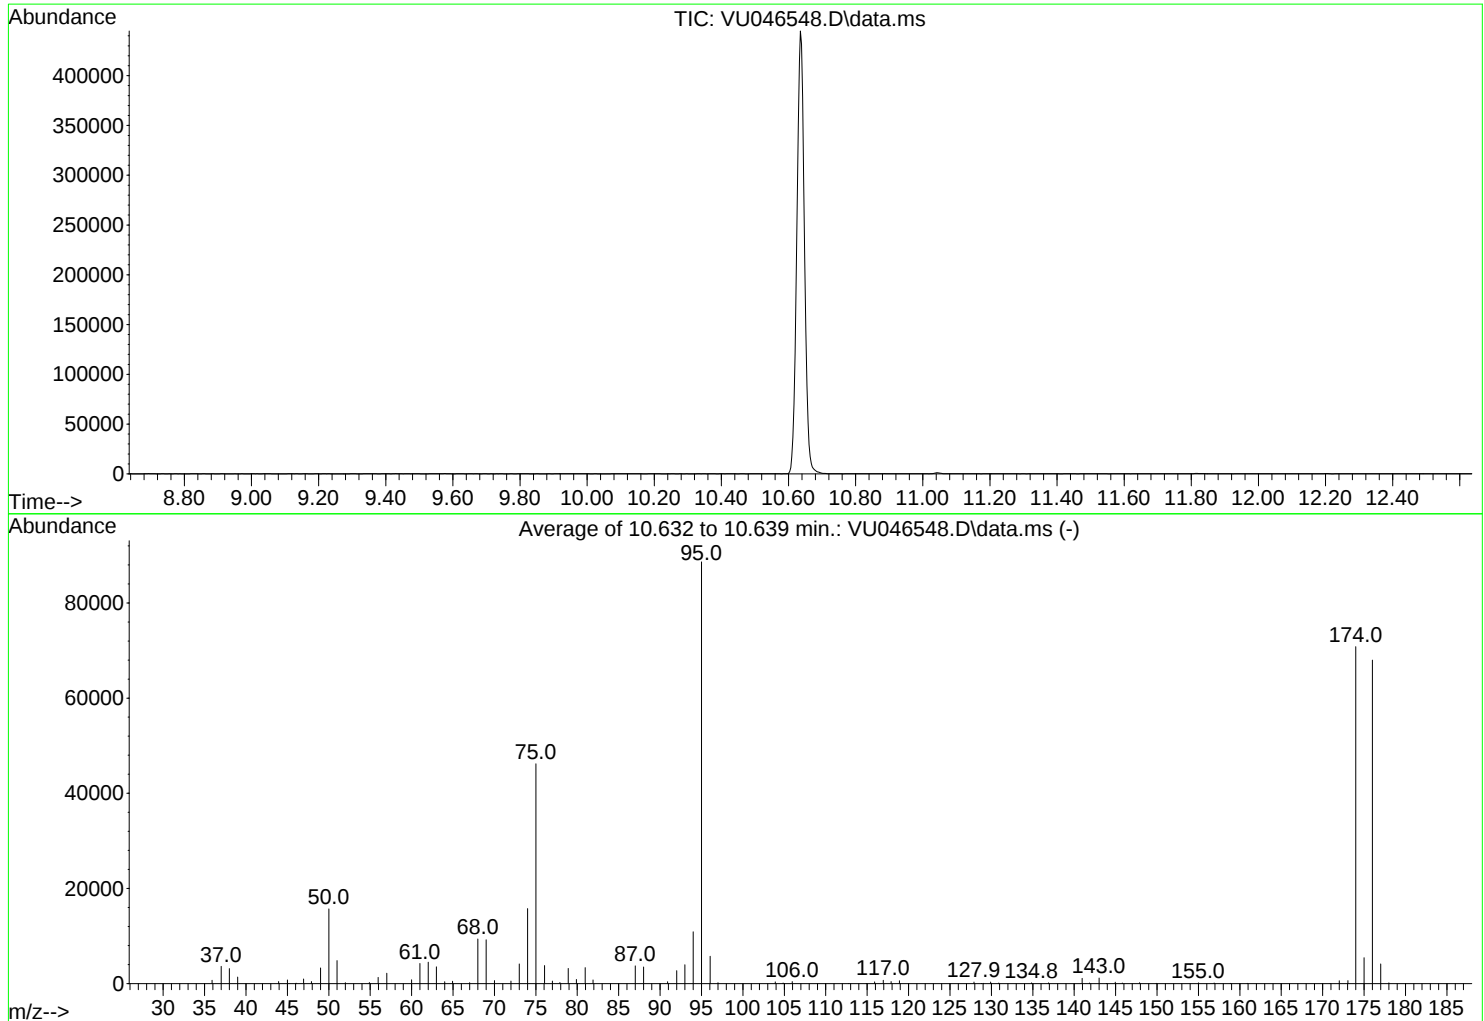

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	15690	PASS
75	95	30	80	52.1	46195	PASS
95	95	100	100	100.0	88637	PASS
96	95	5	9	6.5	5766	PASS
173	174	0.00	2	0.9	645	PASS
174	95	50	120	79.9	70805	PASS
175	174	5	9	7.7	5446	PASS
176	174	95	101	96.0	67995	PASS
177	176	5	9	6.1	4132	PASS

m/z	Abundance
43.90	122.0

Instrument :
MSVOA_U
ClientSampleId :
BFB034

m/z	Abundance
35.00	700.0
37.00	3688.0
38.00	3196.0
39.00	1353.0
44.00	584.0
45.00	697.0
46.00	105.0
47.00	945.0
47.90	461.0
49.00	3346.0
50.00	15461.0
51.00	4785.0
52.00	195.0
54.90	225.0
55.90	1275.0
57.00	2272.0
60.00	770.0
61.00	4062.0
62.00	4481.0
63.00	3496.0
64.00	445.0
64.90	591.0
67.00	203.0
68.00	9229.0
69.00	8827.0
70.00	629.0
72.00	536.0
73.00	4157.0
74.00	15127.0
75.00	44800.0
76.00	3790.0
77.00	514.0
77.90	212.0
78.90	3157.0
79.90	866.0
80.90	3184.0
81.90	805.0
87.00	3725.0
88.00	3428.0
90.90	331.0
92.00	2667.0
93.00	3952.0
94.00	10533.0
95.00	85168.0
96.10	5835.0
97.00	225.0
103.90	371.0
104.90	114.0
106.00	388.0
114.90	104.0
115.90	328.0
117.00	695.0
117.90	411.0
118.90	591.0
127.90	366.0
129.10	105.0
129.90	314.0
130.90	120.0
134.90	163.0
136.90	162.0
140.90	1041.0
141.90	154.0
143.00	1152.0
144.90	322.0
145.80	120.0
147.90	191.0
155.00	178.0
156.90	154.0
172.00	610.0
173.00	574.0
174.00	66960.0
175.00	5111.0
176.00	64000.0
177.00	4033.0
178.00	173.0

Instrument :
MSVOA_U
ClientSampleId :
BFB034

m/z	Abundance
35.90	720.0
37.00	3728.0
38.00	3243.0
39.00	1409.0
44.00	596.0
45.00	796.0
46.10	105.0
46.90	1018.0
47.90	473.0
49.00	3368.0
50.00	16213.0
51.00	4982.0
52.00	203.0
54.90	241.0
55.90	1395.0
57.00	2216.0
60.00	834.0
61.00	4368.0
62.00	4608.0
63.00	3663.0
64.00	429.0
65.00	530.0
67.00	212.0
68.00	9760.0
69.00	9544.0
70.00	667.0
72.00	572.0
73.00	4274.0
74.00	16292.0
75.00	47784.0
76.00	3869.0
77.00	554.0
77.90	226.0
78.90	3327.0
79.90	892.0
80.90	3486.0
81.90	785.0
87.00	3799.0
88.00	3602.0
90.90	417.0
92.00	2870.0
93.00	4129.0
94.00	11258.0
95.00	91888.0
96.10	5915.0
97.00	224.0
103.90	390.0
104.90	137.0
105.90	448.0
112.80	115.0
115.90	376.0
116.90	743.0
117.90	483.0
118.90	640.0
127.90	360.0
129.00	100.0
129.90	361.0
130.90	155.0
134.80	163.0
136.90	189.0
141.00	1143.0
141.80	146.0
143.00	1214.0
143.90	103.0
144.90	315.0
145.80	129.0
147.90	211.0
149.90	111.0
155.00	168.0
156.90	127.0
158.90	118.0
160.90	103.0
170.90	111.0
172.00	616.0
173.00	679.0
174.00	73072.0
175.00	5626.0
176.00	70296.0
177.00	4200.0
178.00	201.0

Instrument :
MSVOA_U
ClientSampleId :
BFB034

m/z	Abundance
35.90	669.0
37.00	3435.0
38.00	3080.0
39.00	1340.0
44.00	551.0
45.00	792.0
46.10	104.0
46.90	987.0
47.90	414.0
49.00	3211.0
50.00	15395.0
51.00	4743.0
52.00	190.0
54.90	245.0
56.00	1307.0
57.00	2073.0
60.00	840.0
61.00	4275.0
62.00	4395.0
63.00	3456.0
64.00	383.0
65.00	437.0
67.00	207.0
68.00	9156.0
69.00	9244.0
70.00	650.0
72.00	500.0
73.00	3981.0
74.00	15860.0
75.00	46000.0
76.10	3714.0
77.00	519.0
77.90	235.0
78.90	3147.0
79.90	846.0
81.00	3457.0
81.90	703.0
87.00	3675.0
88.00	3508.0
90.90	456.0
92.00	2688.0
93.00	3867.0
94.00	10867.0
95.00	88856.0
96.00	5549.0
97.00	172.0
103.90	368.0
104.80	162.0
105.90	461.0
115.90	384.0
116.90	728.0
117.90	464.0
118.90	621.0
127.90	309.0
128.80	109.0
129.90	351.0
130.90	184.0
134.80	149.0
136.90	172.0
141.00	1141.0
141.90	115.0
143.00	1167.0
145.00	291.0
145.80	139.0
147.90	209.0
149.90	127.0
155.00	178.0
156.90	120.0
158.80	137.0
160.90	112.0
172.00	593.0
173.10	683.0
174.00	72384.0
175.00	5600.0
176.00	69688.0
177.00	4162.0
178.00	182.0

Instrument :
MSVOA_U
ClientSampleId :
BFB034