

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
 Data File : VU052485.D
 Acq On : 22 Dec 2022 12:44
 Operator : JC/MD
 Sample : N6169-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBQA7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052485.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.598	73	80	93	rVB	104563	117629	12.16%	1.925%
2	1.913	170	178	194	rVB	90310	118813	12.28%	1.945%
3	2.565	369	381	399	rBV	164145	266407	27.55%	4.360%
4	3.044	522	530	542	rVB3	5643	11005	1.14%	0.180%
5	4.642	1010	1027	1065	rBV	106453	409649	42.36%	6.705%
6	5.060	1141	1157	1182	rBV	142456	317219	32.80%	5.192%
7	5.723	1341	1363	1396	rBV2	291216	770720	79.69%	12.615%
8	6.247	1513	1526	1552	rBV	196563	372013	38.46%	6.089%
9	6.687	1649	1663	1685	rBV	194118	379171	39.20%	6.206%
10	7.562	1924	1935	1956	rBV2	81826	147509	15.25%	2.414%
11	7.896	2025	2039	2055	rBV	312233	538552	55.68%	8.815%
12	8.176	2115	2126	2140	rBV	52746	91331	9.44%	1.495%
13	8.633	2255	2268	2303	rBV2	477448	967152	100.00%	15.830%
14	9.414	2499	2511	2533	rBV	283054	472272	48.83%	7.730%
15	10.752	2913	2927	2942	rBV	153756	247088	25.55%	4.044%
16	10.890	2959	2970	2981	rVB2	8083	12382	1.28%	0.203%
17	11.809	3244	3256	3276	rBV	247453	393447	40.68%	6.440%
18	12.189	3361	3374	3399	rBV	284461	465063	48.09%	7.612%
19	13.838	3878	3887	3900	rBV2	7830	12314	1.27%	0.202%




Sum of corrected areas: 6109736

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
Data File : VU052485.D
Acq On : 22 Dec 2022 12:44
Operator : JC/MD
Sample : N6169-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBQA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

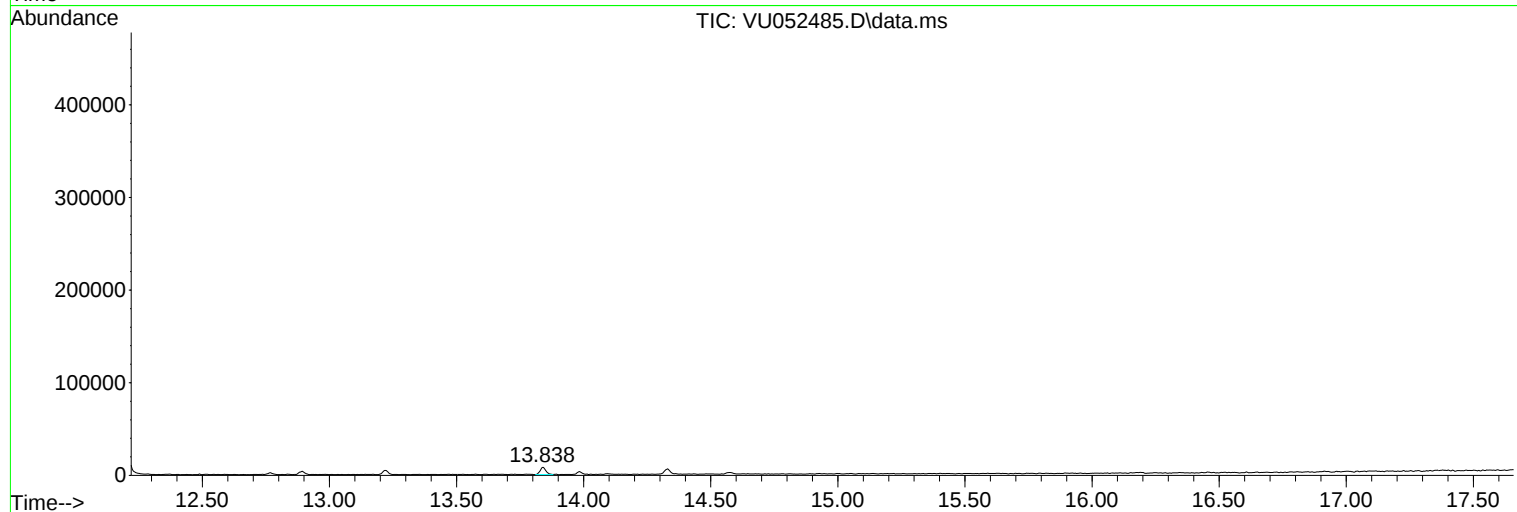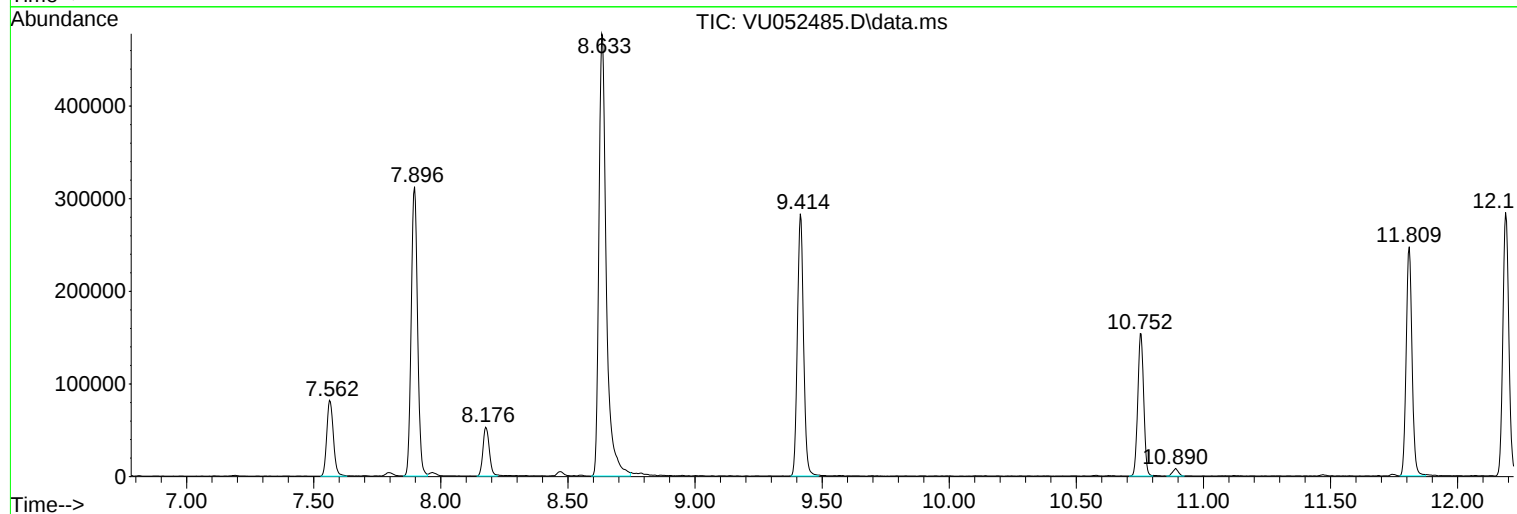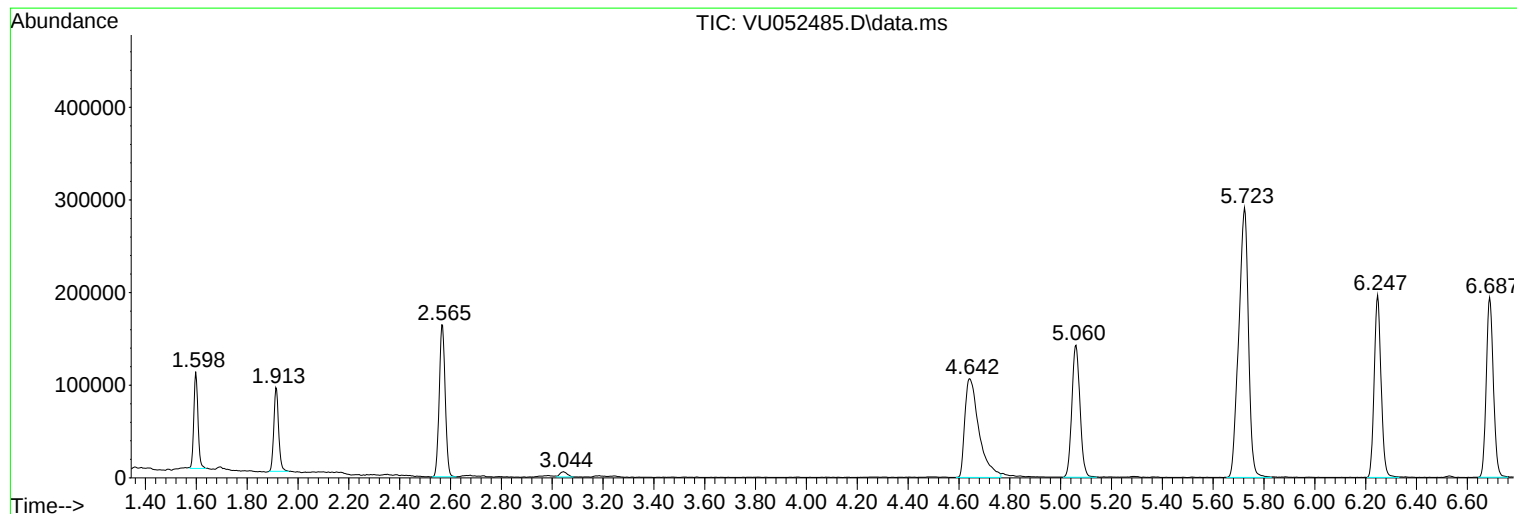

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
Data File : VU052485.D
Acq On : 22 Dec 2022 12:44
Operator : JC/MD
Sample : N6169-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBQA7










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.562	1.98 ug/L	147509	1,4-Difluorobenzene	6.247

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		1,3-Cyclohexadiene	80	C6H8	000592-57-4	25
2		Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	25
3		Thiophosgene	114	CCl2S	000463-71-8	16
4		2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	9
5		2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	9

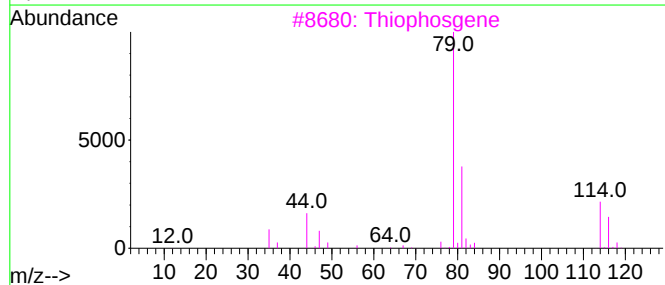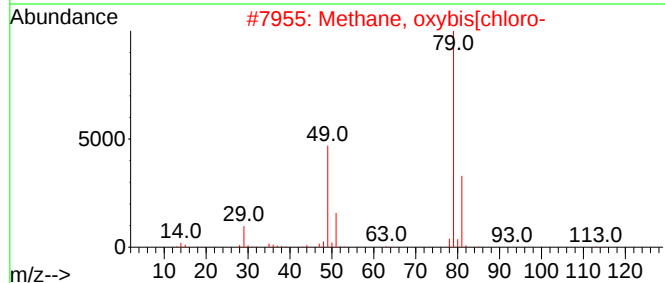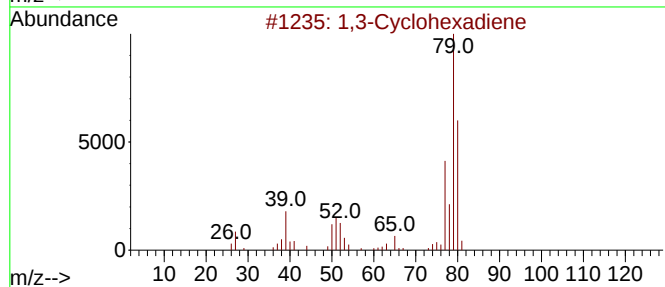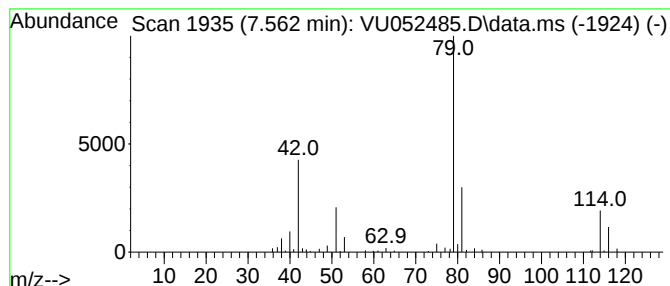

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
Data File : VU052485.D
Acq On : 22 Dec 2022 12:44
Operator : JC/MD
Sample : N6169-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBQA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.562	2.0	ug/L	147509	1	6.247	372013	5.0