

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
 Data File : VU052491.D
 Acq On : 22 Dec 2022 15:05
 Operator : JC/MD
 Sample : N6188-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0L35

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052491.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	95	rVB	109107	124054	10.21%	1.372%
2	1.916	171	179	193	rBV	99254	131313	10.81%	1.452%
3	2.568	370	382	398	rBV	175854	287445	23.66%	3.178%
4	4.639	1012	1026	1077	rBV2	137164	497562	40.95%	5.501%
5	5.079	1141	1163	1184	rBV3	433835	1215089	100.00%	13.434%
6	5.723	1339	1363	1392	rBV2	348937	919103	75.64%	10.162%
7	6.247	1511	1526	1548	rBV	294923	561463	46.21%	6.208%
8	6.687	1645	1663	1682	rBV	225774	442734	36.44%	4.895%
9	7.102	1779	1792	1811	rBV	64350	122359	10.07%	1.353%
10	7.562	1922	1935	1957	rBV	103812	187915	15.47%	2.078%
11	7.896	2024	2039	2053	rBV	395867	687577	56.59%	7.602%
12	7.967	2053	2061	2079	rVB2	23692	42636	3.51%	0.471%
13	8.176	2114	2126	2142	rBV2	66251	113878	9.37%	1.259%
14	8.468	2205	2217	2228	rBV2	8934	16011	1.32%	0.177%
15	8.632	2255	2268	2305	rBV	599774	1174129	96.63%	12.981%
16	8.790	2309	2317	2331	rVB6	8261	18931	1.56%	0.209%
17	9.414	2498	2511	2532	rBV	415976	688154	56.63%	7.608%
18	10.343	2789	2800	2815	rBV4	13160	22472	1.85%	0.248%
19	10.751	2912	2927	2942	rBV	175227	284200	23.39%	3.142%
20	10.890	2960	2970	2983	rVB2	19945	32391	2.67%	0.358%
21	11.471	3141	3151	3167	rBV3	13893	26681	2.20%	0.295%
22	11.806	3243	3255	3277	rBV	411961	659678	54.29%	7.293%
23	12.188	3360	3374	3397	rBV	383242	628462	51.72%	6.948%
24	12.883	3582	3590	3600	rBV4	21622	32815	2.70%	0.363%
25	15.221	4307	4317	4326	rVB6	6867	13388	1.10%	0.148%
26	16.259	4631	4640	4648	rBV2	13394	22256	1.83%	0.246%
27	16.404	4676	4685	4693	rBV2	16094	26262	2.16%	0.290%
28	17.111	4899	4905	4917	rVB3	8606	15458	1.27%	0.171%
29	17.368	4980	4985	5004	rVB7	11340	25449	2.09%	0.281%
30	17.536	5030	5037	5050	rBV6	11154	24936	2.05%	0.276%




Sum of corrected areas: 9044801

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
Data File : VU052491.D
Acq On : 22 Dec 2022 15:05
Operator : JC/MD
Sample : N6188-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COL35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

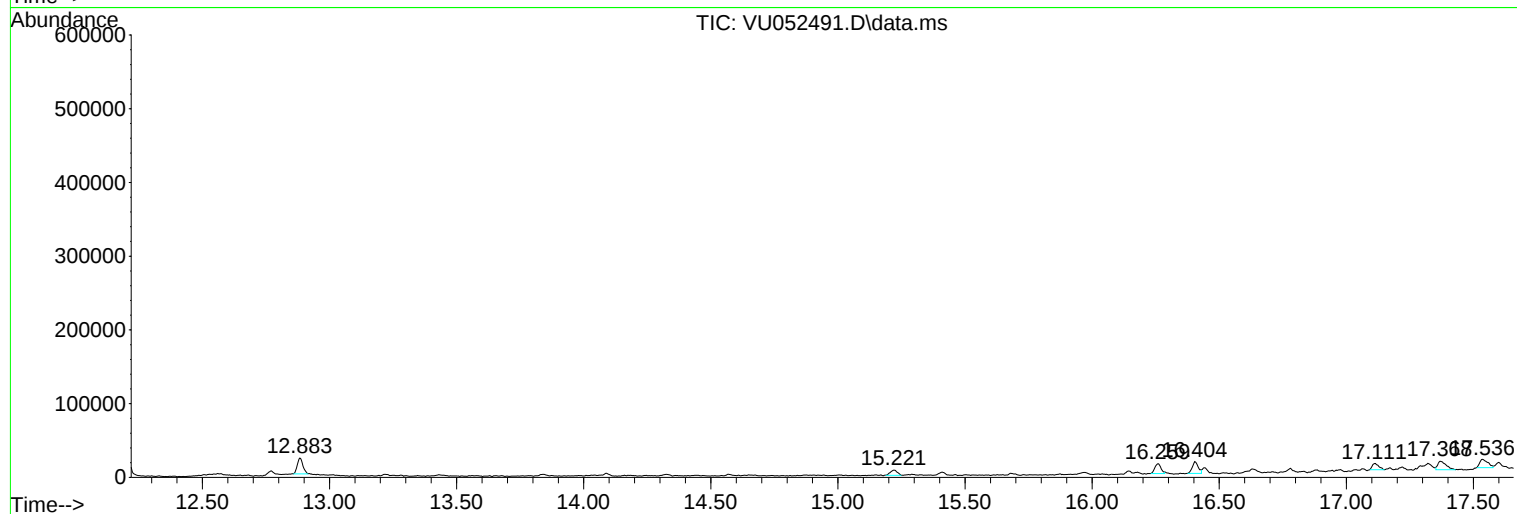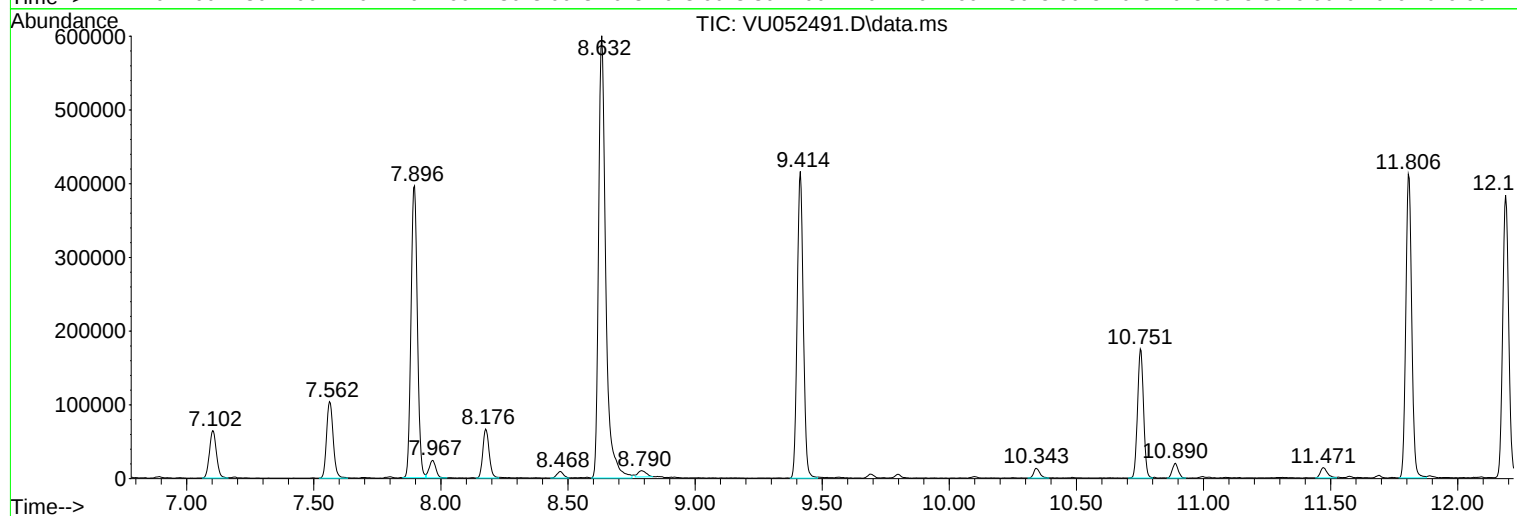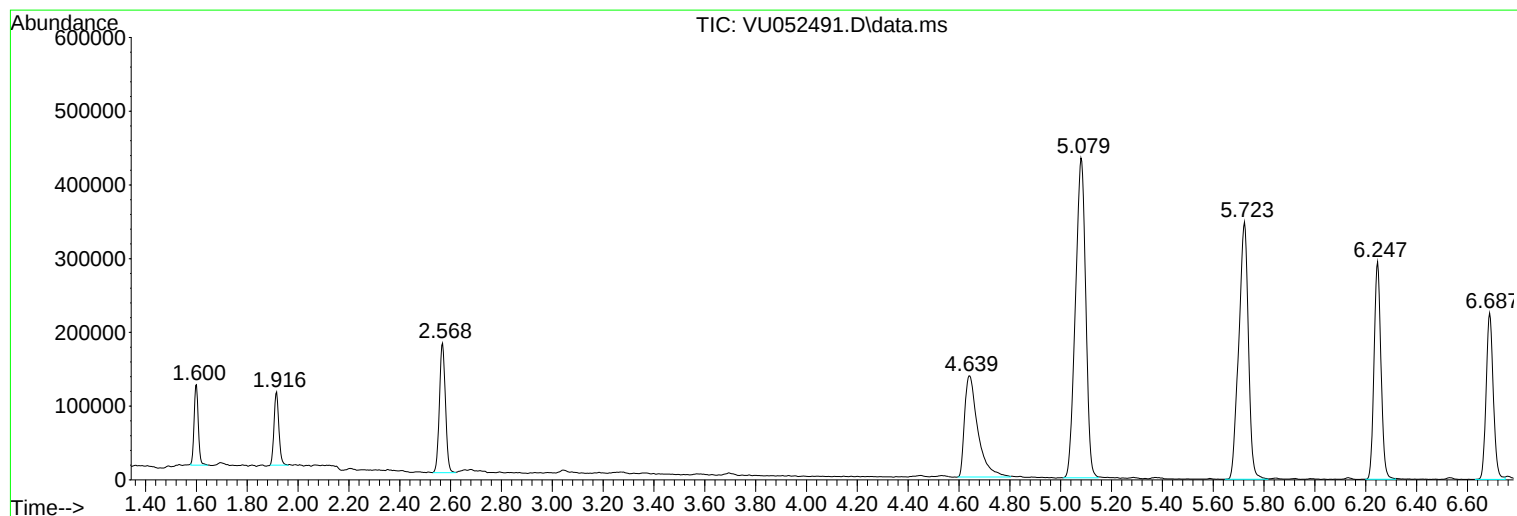

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
Data File : VU052491.D
Acq On : 22 Dec 2022 15:05
Operator : JC/MD
Sample : N6188-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
Data File : VU052491.D
Acq On : 22 Dec 2022 15:05
Operator : JC/MD
Sample : N6188-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc