

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
 Data File : VU052492.D
 Acq On : 22 Dec 2022 15:29
 Operator : JC/MD
 Sample : N6188-13
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COL50

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU052492.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	92	rVB	110440	128810	11.12%	1.565%
2	1.694	105	110	122	rVB2	7411	12704	1.10%	0.154%
3	1.915	170	179	196	rBV	102243	137401	11.87%	1.669%
4	2.568	369	382	397	rBV	176687	290249	25.06%	3.525%
5	2.658	397	410	444	rVB2	7856	30323	2.62%	0.368%
6	4.436	948	963	976	rBV2	7002	17678	1.53%	0.215%
7	4.639	1011	1026	1067	rBV	146045	484038	41.80%	5.879%
8	5.076	1140	1162	1184	rBV4	250969	793952	68.56%	9.644%
9	5.722	1341	1363	1387	rBV2	356029	928901	80.22%	11.283%
10	6.247	1510	1526	1551	rBV	235341	454982	39.29%	5.526%
11	6.687	1648	1663	1680	rBV	227542	443667	38.31%	5.389%
12	7.102	1780	1792	1809	rBV	41201	78397	6.77%	0.952%
13	7.562	1923	1935	1952	rBV	105194	185857	16.05%	2.257%
14	7.896	2024	2039	2054	rBV	408501	701188	60.55%	8.517%
15	7.967	2054	2061	2076	rVB2	16722	27913	2.41%	0.339%
16	8.176	2115	2126	2144	rBV	65482	112038	9.68%	1.361%
17	8.468	2205	2217	2233	rBV2	12811	22918	1.98%	0.278%
18	8.632	2255	2268	2308	rBV	594202	1157994	100.00%	14.065%
19	8.787	2308	2316	2331	rVB5	11315	23536	2.03%	0.286%
20	9.414	2499	2511	2535	rBV	340901	563202	48.64%	6.841%
21	9.796	2621	2630	2641	rBV3	7618	12296	1.06%	0.149%
22	10.343	2790	2800	2817	rVB5	11794	19558	1.69%	0.238%
23	10.751	2914	2927	2945	rBV	178193	289037	24.96%	3.511%
24	10.889	2959	2970	2983	rVB2	26739	44848	3.87%	0.545%
25	11.471	3140	3151	3167	rBV3	16512	31919	2.76%	0.388%
26	11.809	3242	3256	3275	rBV	334682	541685	46.78%	6.580%
27	12.188	3360	3374	3398	rBV	387406	630082	54.41%	7.653%
28	12.767	3541	3554	3563	rBV	8396	13010	1.12%	0.158%
29	12.883	3581	3590	3604	rBV4	25739	41813	3.61%	0.508%
30	16.256	4631	4639	4652	rBV4	7217	12881	1.11%	0.156%




Sum of corrected areas: 8232877

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
Data File : VU052492.D
Acq On : 22 Dec 2022 15:29
Operator : JC/MD
Sample : N6188-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COL50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

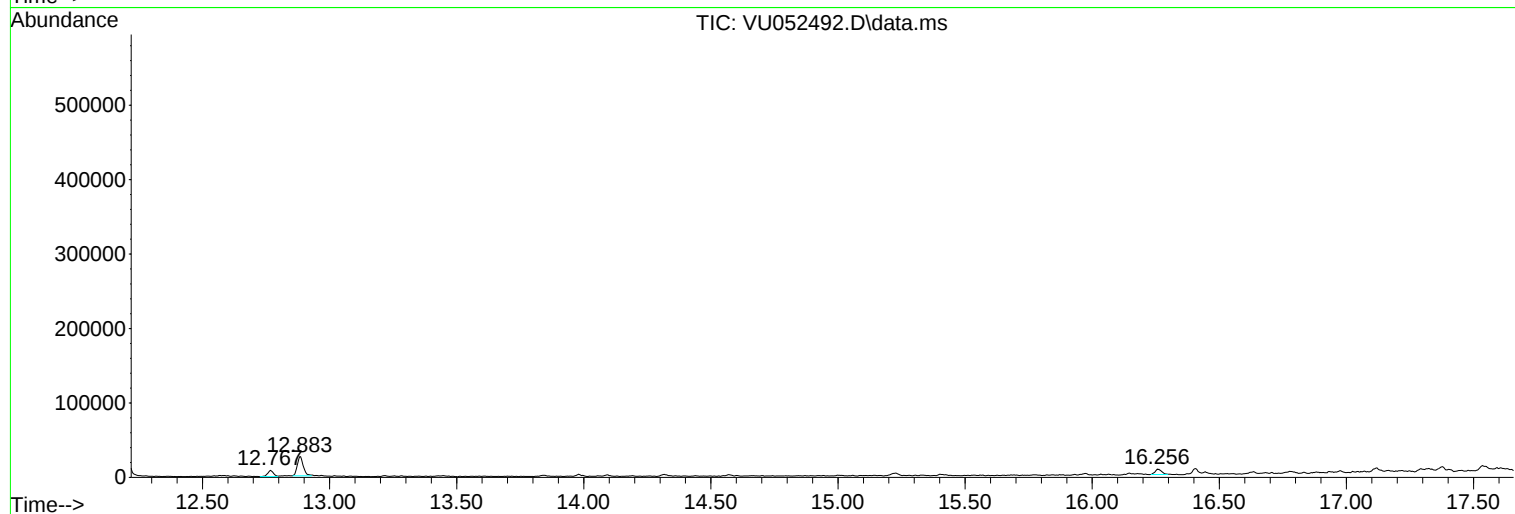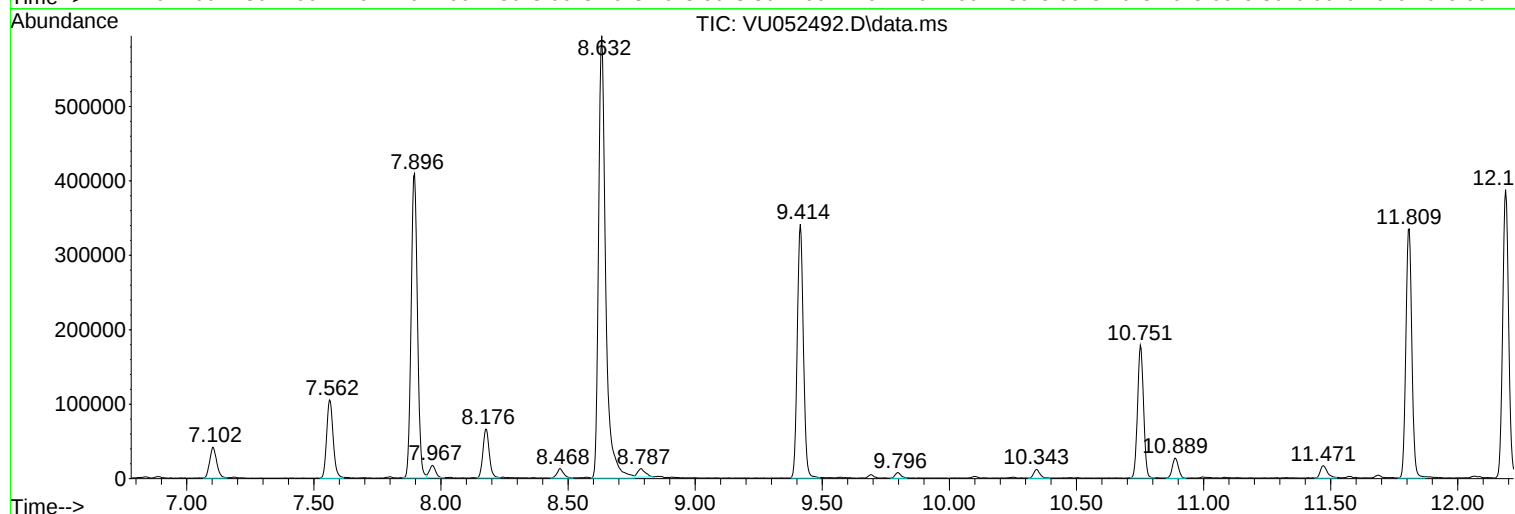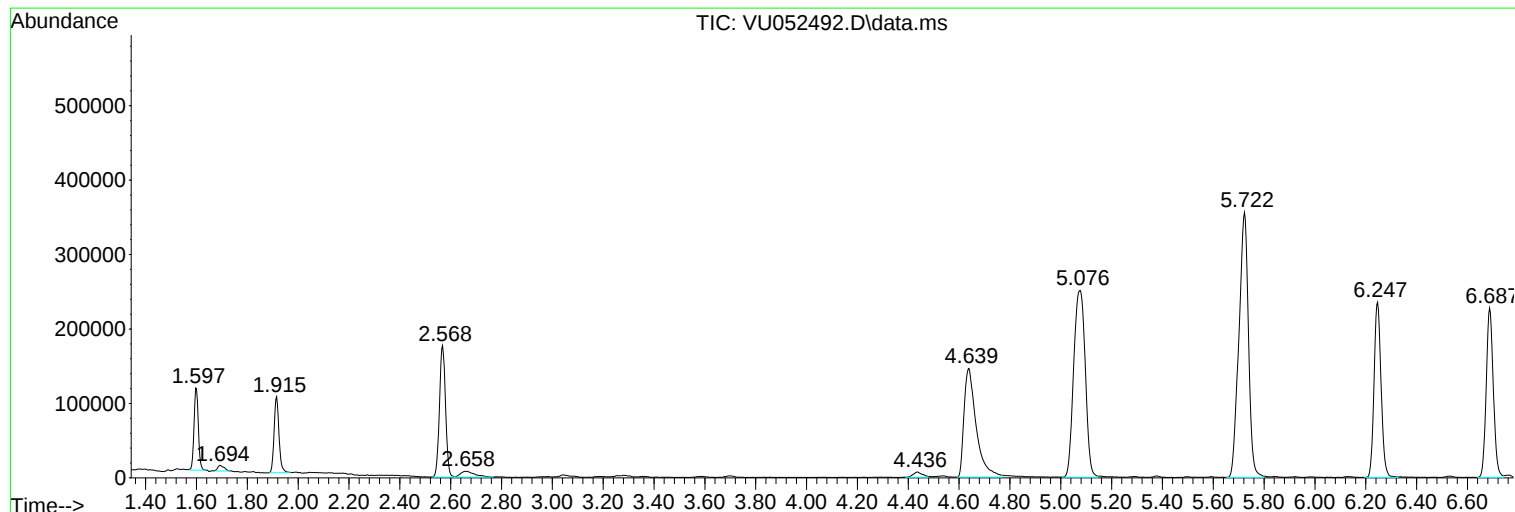

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
Data File : VU052492.D
Acq On : 22 Dec 2022 15:29
Operator : JC/MD
Sample : N6188-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
Data File : VU052492.D
Acq On : 22 Dec 2022 15:29
Operator : JC/MD
Sample : N6188-13
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc