

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
 Data File : VU052494.D
 Acq On : 22 Dec 2022 16:16
 Operator : JC/MD
 Sample : N6188-02 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0L36

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052494.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	91	rVB	117138	135429	9.33%	1.378%
2	1.916	170	179	197	rBV	109854	147794	10.18%	1.504%
3	2.568	370	382	399	rVB	190888	310066	21.37%	3.154%
4	3.044	520	530	543	rBV4	21638	41496	2.86%	0.422%
5	4.645	1011	1028	1080	rBV2	171526	656264	45.22%	6.677%
6	5.060	1141	1157	1177	rBV	180633	397817	27.41%	4.047%
7	5.723	1342	1363	1393	rBV2	384821	1002473	69.08%	10.199%
8	6.247	1511	1526	1550	rBV	294010	556365	38.34%	5.660%
9	6.539	1602	1617	1638	rBV	777990	1451256	100.00%	14.764%
10	6.687	1648	1663	1680	rBV	251191	484539	33.39%	4.929%
11	7.562	1923	1935	1955	rBV	115041	206991	14.26%	2.106%
12	7.896	2025	2039	2056	rBV	447143	770680	53.10%	7.841%
13	8.176	2116	2126	2142	rBV	70173	119814	8.26%	1.219%
14	8.632	2255	2268	2302	rBV	640283	1234203	85.04%	12.556%
15	9.414	2498	2511	2535	rBV	404442	676693	46.63%	6.884%
16	10.751	2913	2927	2943	rBV	188126	307916	21.22%	3.133%
17	10.890	2958	2970	2982	rVB	11966	19852	1.37%	0.202%
18	11.809	3243	3256	3278	rBV	396312	628874	43.33%	6.398%
19	12.189	3361	3374	3397	rBV	421407	680897	46.92%	6.927%




Sum of corrected areas: 9829419

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
Data File : VU052494.D
Acq On : 22 Dec 2022 16:16
Operator : JC/MD
Sample : N6188-02 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COL36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

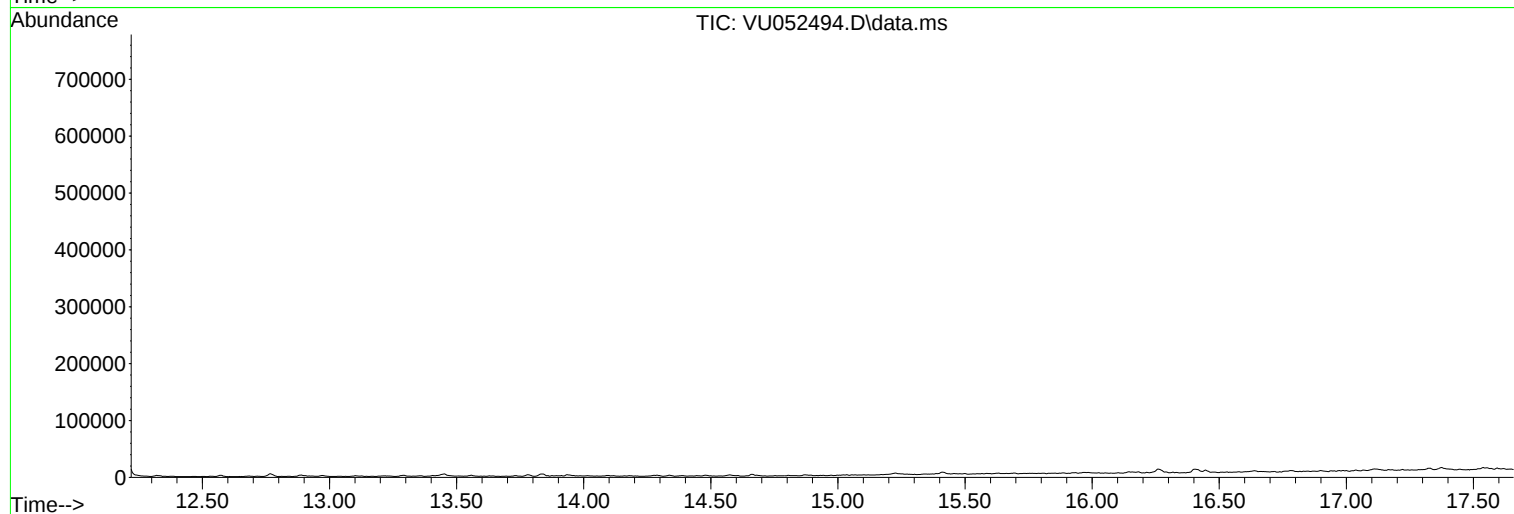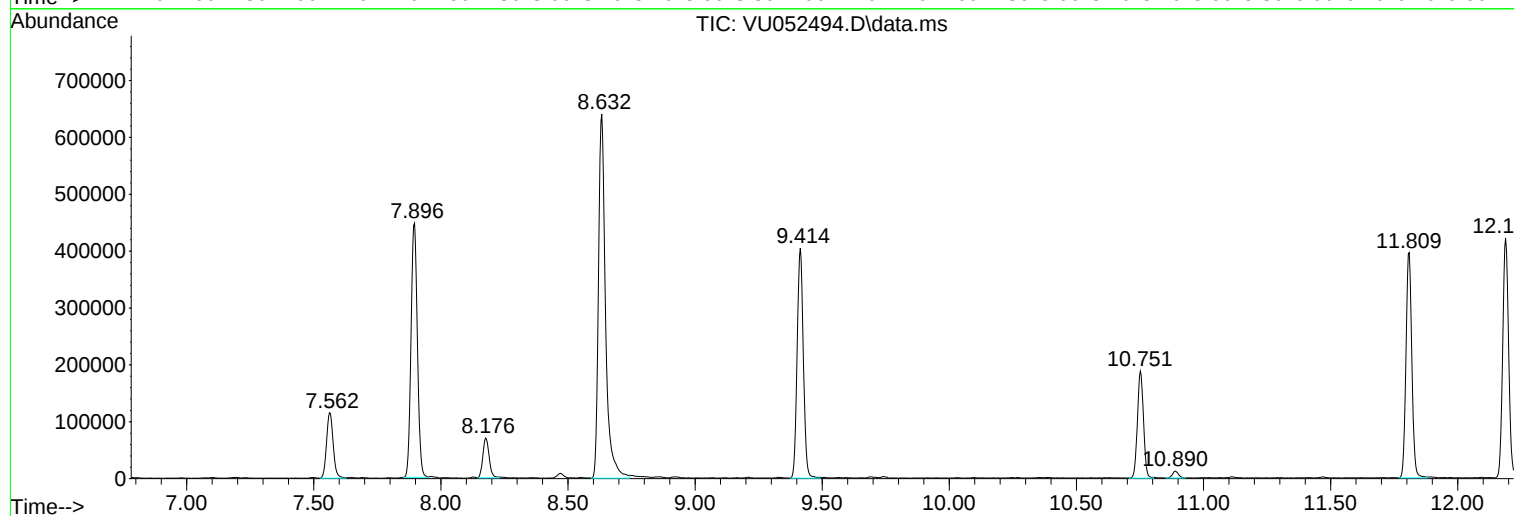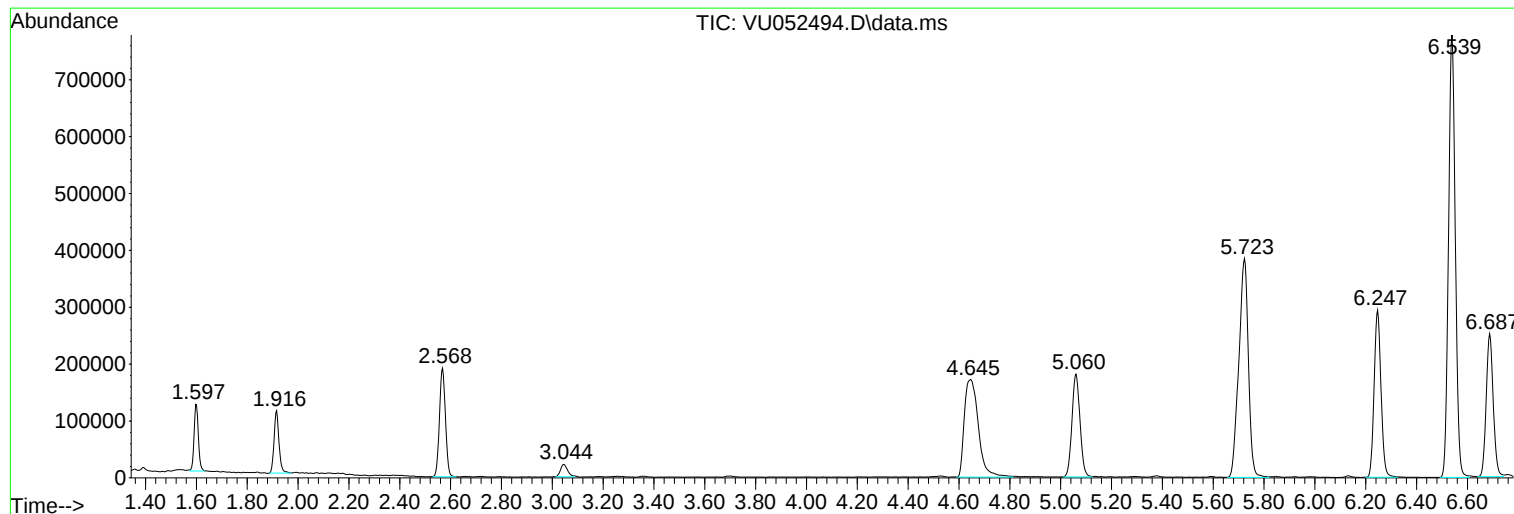

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
Data File : VU052494.D
Acq On : 22 Dec 2022 16:16
Operator : JC/MD
Sample : N6188-02 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
Data File : VU052494.D
Acq On : 22 Dec 2022 16:16
Operator : JC/MD
Sample : N6188-02 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L36

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
