

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
 Data File : VU052495.D
 Acq On : 22 Dec 2022 16:39
 Operator : JC/MD
 Sample : N6188-03 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0L37

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052495.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	96	rVB	115602	134061	9.48%	1.436%
2	1.916	170	179	193	rBV	105015	138576	9.80%	1.485%
3	2.568	369	382	405	rVB	184127	302368	21.39%	3.240%
4	3.047	520	531	549	rVB2	14271	30716	2.17%	0.329%
5	4.655	1012	1031	1083	rBV2	166765	644761	45.60%	6.908%
6	5.060	1137	1157	1180	rBV	170334	379963	26.88%	4.071%
7	5.722	1341	1363	1391	rBV2	361695	951307	67.29%	10.192%
8	6.247	1508	1526	1549	rBV	270344	511754	36.20%	5.483%
9	6.539	1602	1617	1646	rBV	752879	1413802	100.00%	15.147%
10	6.687	1646	1663	1680	rBV	234511	458173	32.41%	4.909%
11	7.562	1923	1935	1953	rBV	111320	195592	13.83%	2.096%
12	7.896	2026	2039	2057	rBV	416604	724290	51.23%	7.760%
13	8.176	2115	2126	2142	rBV	68008	115792	8.19%	1.241%
14	8.632	2255	2268	2315	rBV	602249	1201540	84.99%	12.873%
15	9.414	2498	2511	2534	rBV	376825	620141	43.86%	6.644%
16	10.751	2915	2927	2941	rBV	178447	291855	20.64%	3.127%
17	10.889	2960	2970	2986	rVB	7755	14282	1.01%	0.153%
18	11.809	3244	3256	3278	rBV	347808	567157	40.12%	6.076%
19	12.188	3360	3374	3396	rBV	392514	637538	45.09%	6.831%




Sum of corrected areas: 9333668

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
Data File : VU052495.D
Acq On : 22 Dec 2022 16:39
Operator : JC/MD
Sample : N6188-03 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COL37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

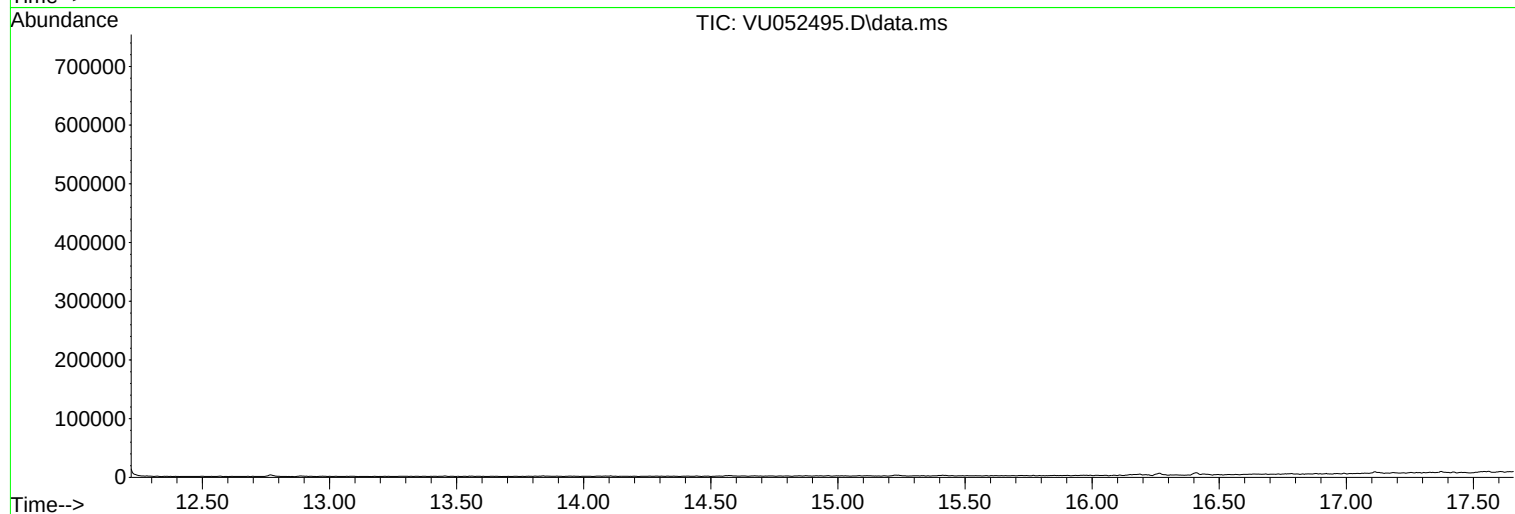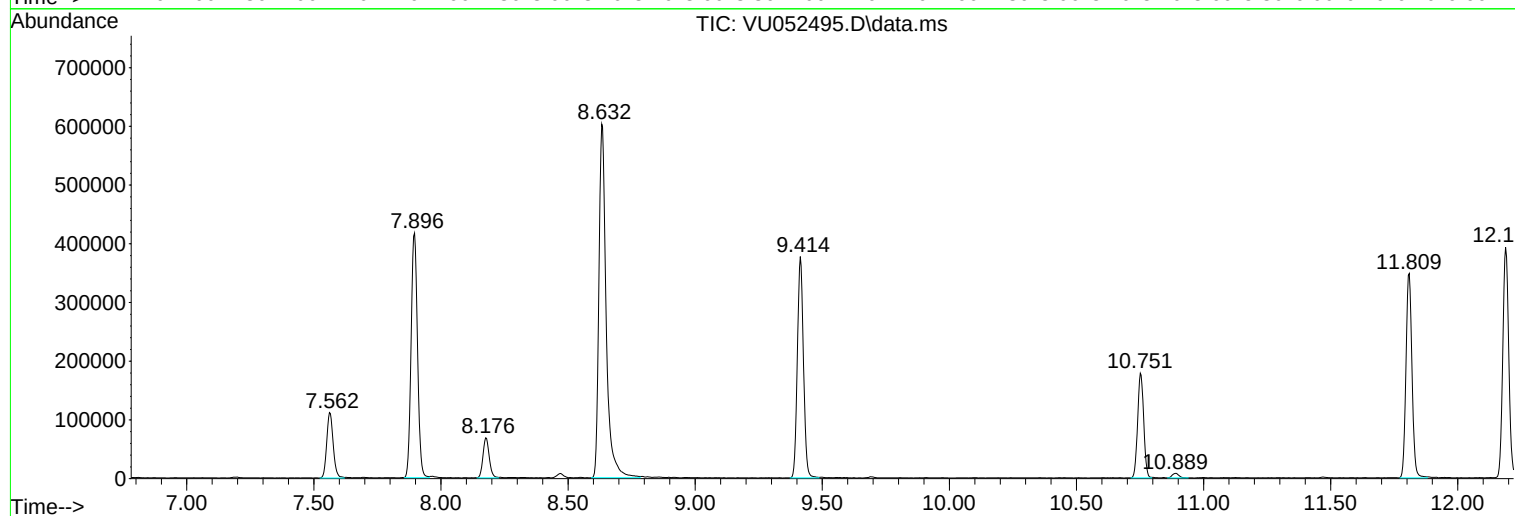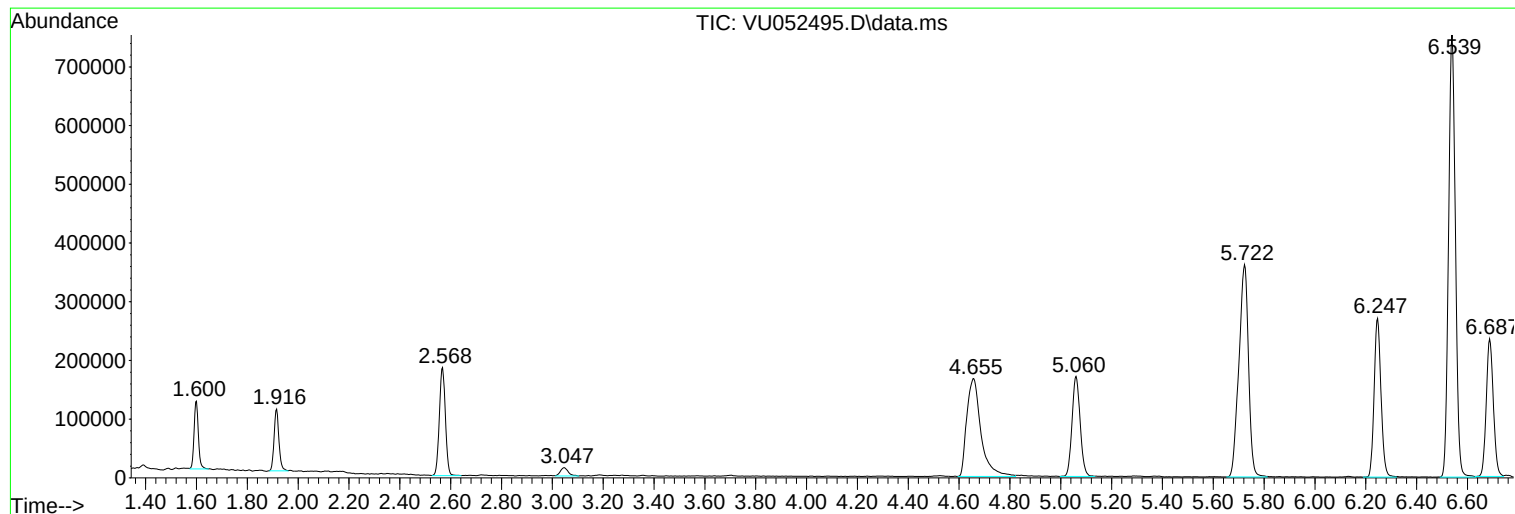

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
Data File : VU052495.D
Acq On : 22 Dec 2022 16:39
Operator : JC/MD
Sample : N6188-03 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
Data File : VU052495.D
Acq On : 22 Dec 2022 16:39
Operator : JC/MD
Sample : N6188-03 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------