

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
 Data File : VU052498.D
 Acq On : 22 Dec 2022 17:50
 Operator : JC/MD
 Sample : N6188-06DL 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0L40DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052498.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	94	rVB	109207	126191	10.36%	1.607%
2	1.912	170	178	196	rVB	97940	131424	10.79%	1.674%
3	2.568	369	382	397	rBV	170079	280290	23.00%	3.569%
4	3.044	518	530	544	rVB	18589	35072	2.88%	0.447%
5	4.655	1007	1031	1074	rBV2	142867	591884	48.57%	7.537%
6	5.060	1140	1157	1182	rBV	158904	351410	28.84%	4.475%
7	5.723	1340	1363	1386	rBV2	340495	891280	73.14%	11.350%
8	6.247	1512	1526	1550	rBV	285901	553968	45.46%	7.054%
9	6.539	1604	1617	1637	rBV	63920	118639	9.74%	1.511%
10	6.687	1649	1663	1682	rBV	221722	432455	35.49%	5.507%
11	7.562	1923	1935	1962	rVB	98288	180531	14.82%	2.299%
12	7.893	2023	2038	2054	rBV	377797	657193	53.93%	8.369%
13	7.967	2054	2061	2074	rVB	6872	13248	1.09%	0.169%
14	8.176	2114	2126	2145	rBV	63371	110827	9.10%	1.411%
15	8.632	2254	2268	2308	rBV	612101	1218524	100.00%	15.517%
16	9.414	2498	2511	2534	rBV	410212	675067	55.40%	8.597%
17	10.751	2916	2927	2943	rVB	181618	289037	23.72%	3.681%
18	11.809	3239	3256	3276	rBV	369121	606130	49.74%	7.719%
19	12.189	3358	3374	3401	rBV	358402	589596	48.39%	7.508%




Sum of corrected areas: 7852766

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
Data File : VU052498.D
Acq On : 22 Dec 2022 17:50
Operator : JC/MD
Sample : N6188-06DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L40DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

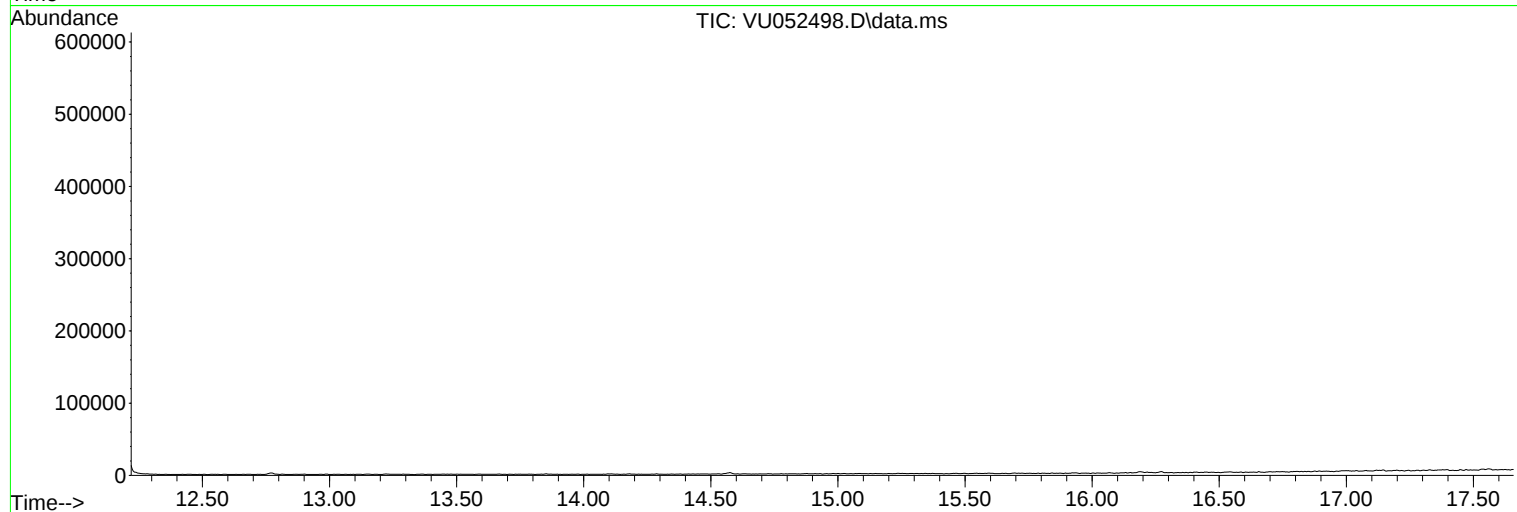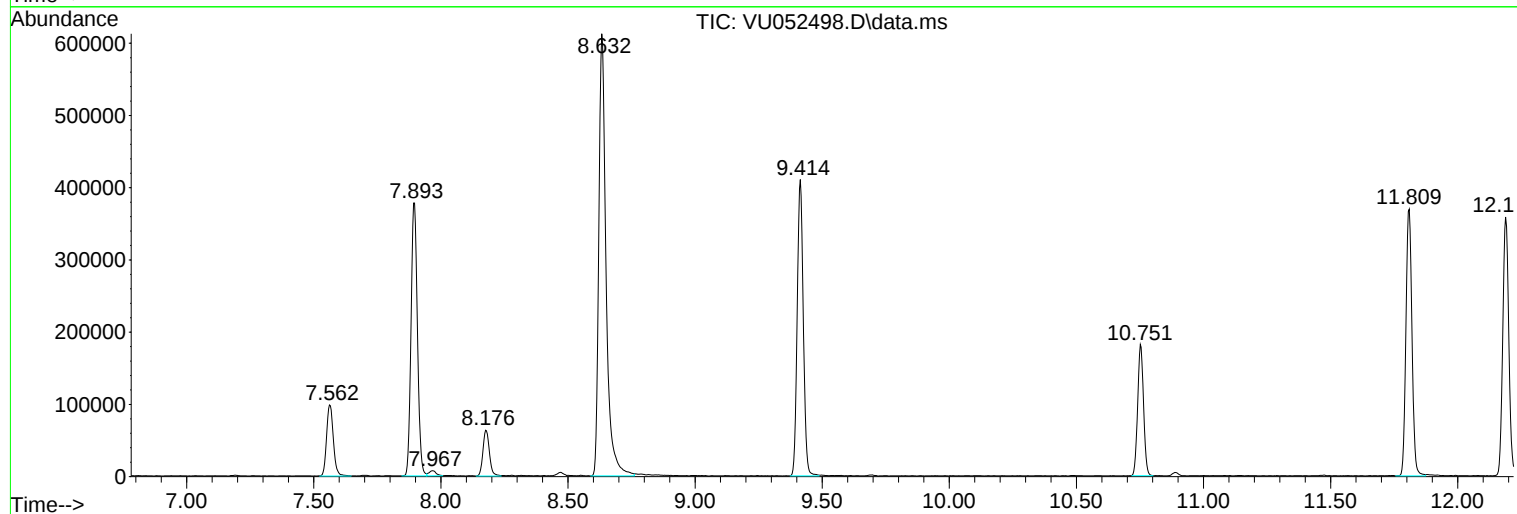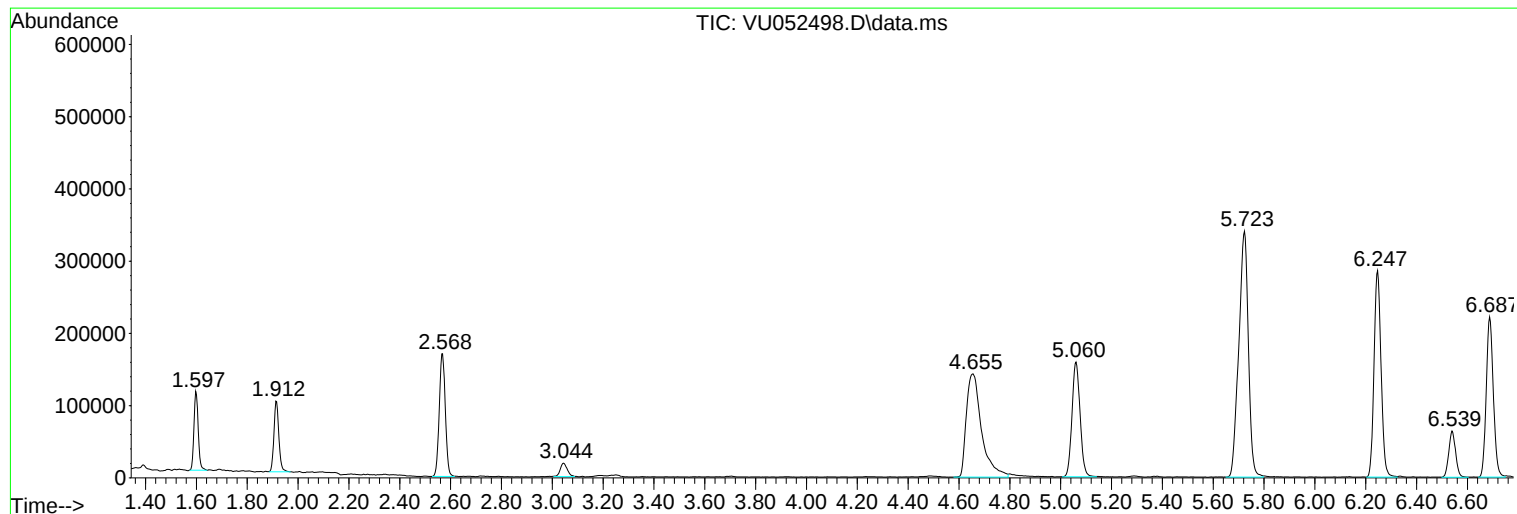

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
Data File : VU052498.D
Acq On : 22 Dec 2022 17:50
Operator : JC/MD
Sample : N6188-06DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L40DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
Data File : VU052498.D
Acq On : 22 Dec 2022 17:50
Operator : JC/MD
Sample : N6188-06DL 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L40DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc