

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
 Data File : VU052505.D
 Acq On : 22 Dec 2022 20:31
 Operator : JC/MD
 Sample : N6189-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0L42

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU052505.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rBV	98517	115043	10.06%	1.687%
2	1.912	170	178	193	rVB	87020	117038	10.23%	1.716%
3	2.568	370	382	398	rBV	157028	258569	22.61%	3.792%
4	4.655	1009	1031	1087	rBV	92468	482725	42.20%	7.079%
5	5.060	1139	1157	1181	rBV	146345	327858	28.66%	4.808%
6	5.723	1342	1363	1389	rBV2	307275	810299	70.84%	11.884%
7	6.247	1508	1526	1551	rBV	228206	437947	38.29%	6.423%
8	6.687	1649	1663	1680	rBV	200188	396786	34.69%	5.819%
9	7.562	1923	1935	1953	rBV	88775	159040	13.90%	2.332%
10	7.893	2020	2038	2056	rBV	333167	582473	50.92%	8.542%
11	8.176	2114	2126	2140	rBV	58521	100402	8.78%	1.472%
12	8.472	2205	2218	2229	rVB3	6213	11495	1.00%	0.169%
13	8.636	2253	2269	2309	rBV	542103	1143787	100.00%	16.774%
14	9.414	2495	2511	2535	rBV	328951	548571	47.96%	8.045%
15	10.751	2915	2927	2942	rBV	169122	275747	24.11%	4.044%
16	10.890	2959	2970	2985	rVB3	12288	19467	1.70%	0.285%
17	11.806	3243	3255	3276	rBV	293116	472465	41.31%	6.929%
18	12.189	3362	3374	3395	rBV	323184	523330	45.75%	7.675%
19	15.343	4347	4355	4373	rVB3	20757	35591	3.11%	0.522%




Sum of corrected areas: 6818633

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
Data File : VU052505.D
Acq On : 22 Dec 2022 20:31
Operator : JC/MD
Sample : N6189-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COL42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

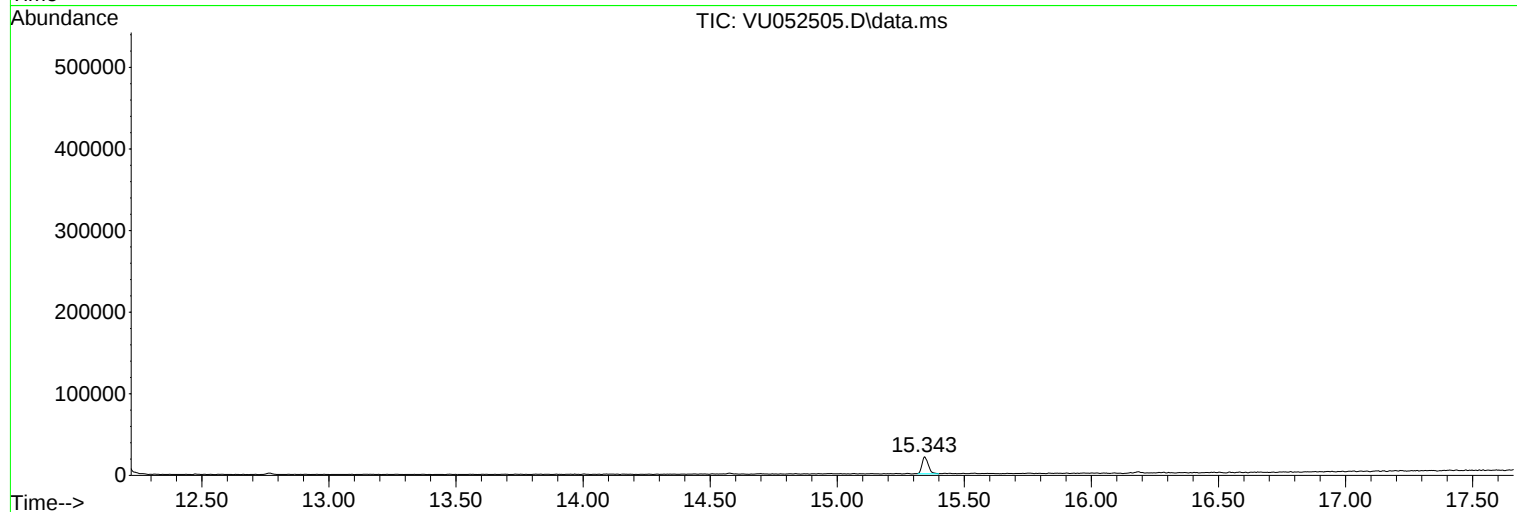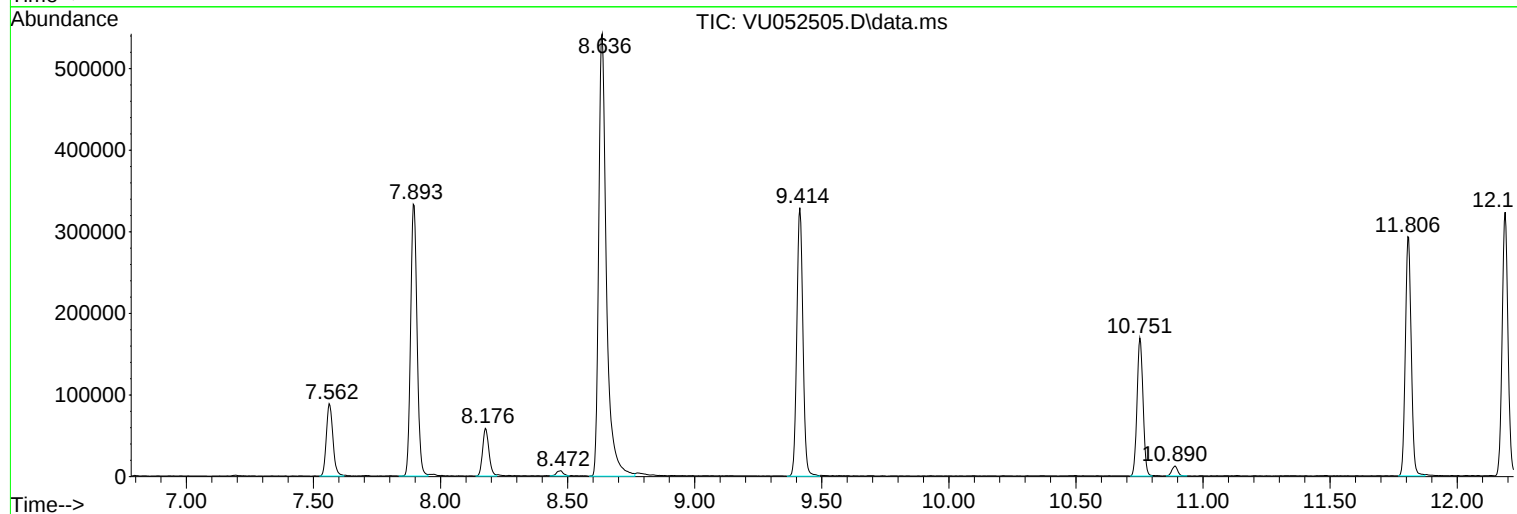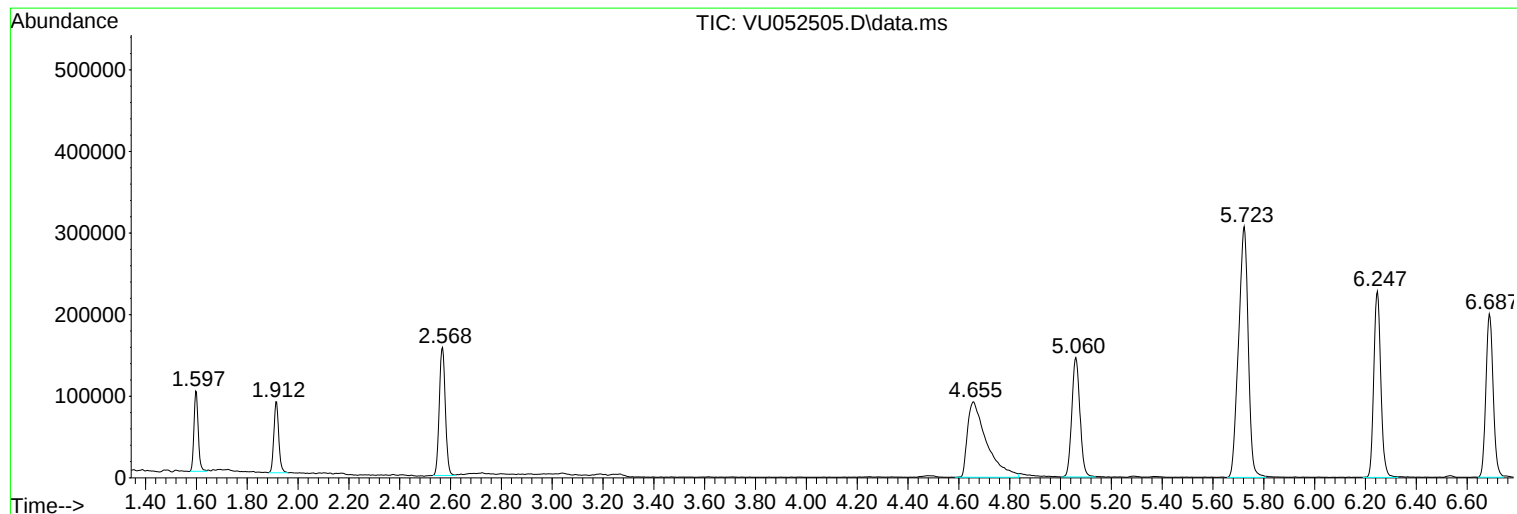

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
Data File : VU052505.D
Acq On : 22 Dec 2022 20:31
Operator : JC/MD
Sample : N6189-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
Data File : VU052505.D
Acq On : 22 Dec 2022 20:31
Operator : JC/MD
Sample : N6189-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------