


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122222\
 Data File : VU052481.D
 Acq On : 22 Dec 2022 09:58
 Operator : JC/MD
 Sample : BFB183
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB183

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Dec 28 01:18:16 2022

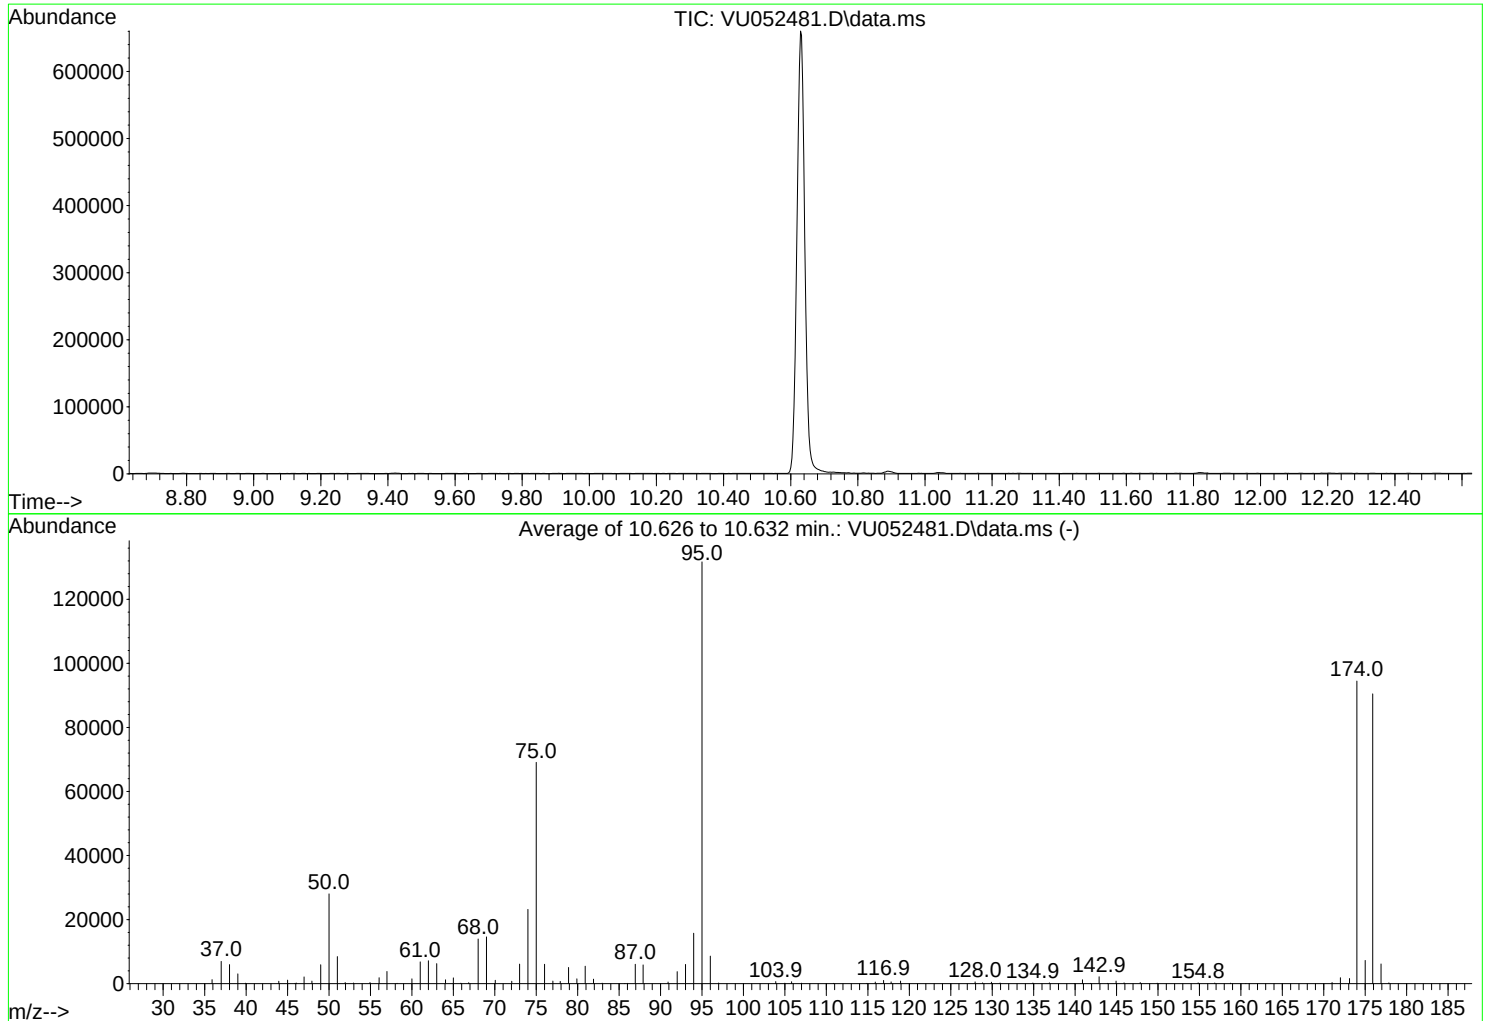

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	28045	PASS
75	95	30	80	52.5	69075	PASS
95	95	100	100	100.0	131691	PASS
96	95	5	9	6.5	8591	PASS
173	174	0.00	2	1.7	1603	PASS
174	95	50	120	71.7	94448	PASS
175	174	5	9	7.7	7258	PASS
176	174	95	101	95.8	90461	PASS
177	176	5	9	6.8	6162	PASS

m/z	Abundance
39.90	258.0
43.90	432.0

Instrument :
MSVOA_U
ClientSampleId :
BFB183

m/z	Abundance
35.90	1141.0
37.00	6587.0
38.00	5750.0
39.00	3045.0
40.10	393.0
44.00	1097.0
45.00	1121.0
45.90	240.0
47.00	1981.0
48.00	861.0
49.00	5467.0
50.00	27000.0
51.00	8343.0
52.00	437.0
52.90	189.0
55.00	340.0
56.00	1763.0
57.00	3590.0
58.20	151.0
60.00	1567.0
61.00	6248.0
62.00	6796.0
63.00	6157.0
64.10	1209.0
65.00	1801.0
65.90	177.0
66.90	285.0
68.00	13627.0
69.00	14029.0
70.10	1068.0
72.00	738.0
73.00	5714.0
74.00	21808.0
75.00	66464.0
76.00	5744.0
77.00	749.0
77.90	666.0
78.90	4865.0
79.90	1376.0
80.90	5367.0
81.90	1404.0
82.90	148.0
86.00	165.0
87.00	5667.0
87.90	5310.0
90.90	515.0
92.00	3643.0
93.00	5857.0
94.00	15336.0
95.00	125056.0
96.00	8046.0
97.00	183.0
103.90	682.0
105.00	157.0
105.80	592.0
107.00	104.0
110.80	113.0
114.90	109.0
115.90	499.0
116.90	973.0
117.80	523.0
118.90	762.0
128.00	366.0
128.80	278.0
129.90	373.0
130.90	145.0
134.90	160.0
136.90	179.0
139.90	116.0
140.90	1178.0
142.90	2090.0
145.00	849.0
145.90	288.0
147.80	365.0
149.90	110.0
154.80	206.0
156.80	186.0
158.80	145.0
160.60	128.0
171.00	376.0
172.00	1767.0
173.10	1626.0
174.00	87520.0
175.00	6661.0
175.90	84152.0
176.90	5739.0
177.90	222.0

Instrument :
MSVOA_U
ClientSampleId :
BFB183

m/z	Abundance
35.90	1248.0
37.00	7219.0
38.00	6142.0
39.00	3232.0
40.10	412.0
44.00	1188.0
45.00	1143.0
46.10	286.0
47.00	2171.0
47.90	818.0
49.00	6125.0
50.00	29096.0
51.00	8679.0
51.90	382.0
52.90	199.0
54.90	391.0
56.00	1896.0
57.00	3910.0
58.20	116.0
60.00	1554.0
61.00	6961.0
62.00	7375.0
63.00	6398.0
64.00	1226.0
65.00	1827.0
65.90	177.0
66.90	328.0
68.00	14381.0
69.00	15076.0
70.00	1142.0
72.10	787.0
73.00	6318.0
74.00	23912.0
75.00	71344.0
76.00	6136.0
77.00	844.0
77.90	762.0
78.90	5203.0
79.90	1557.0
80.90	5569.0
81.90	1412.0
82.90	150.0
86.00	171.0
86.90	6208.0
87.90	6008.0
90.90	518.0
92.00	3808.0
93.00	6142.0
94.00	16284.0
95.00	135680.0
96.00	8866.0
97.00	207.0
103.90	658.0
105.00	163.0
105.80	607.0
107.00	129.0
110.80	114.0
114.90	117.0
115.90	512.0
116.90	1037.0
117.80	545.0
119.00	837.0
128.00	411.0
128.80	287.0
129.90	452.0
131.00	184.0
134.90	204.0
136.90	253.0
140.90	1246.0
141.90	139.0
142.90	2190.0
143.90	127.0
144.90	853.0
145.90	260.0
147.90	348.0
149.90	137.0
154.90	255.0
156.90	231.0
158.70	141.0
160.60	103.0
171.00	349.0
172.00	1918.0
173.10	1659.0
174.00	97288.0
175.00	7594.0
175.90	93304.0
176.90	6403.0
177.80	263.0

Instrument :
MSVOA_U
ClientSampleId :
BFB183

m/z	Abundance
35.90	1335.0
37.00	7078.0
38.00	5983.0
39.00	2939.0
40.00	371.0
44.00	1218.0
45.00	1076.0
46.00	282.0
47.00	2158.0
47.90	778.0
49.00	6134.0
50.00	28040.0
51.00	8287.0
51.90	310.0
53.00	190.0
54.90	379.0
56.10	1841.0
57.00	3946.0
60.00	1411.0
61.00	7142.0
62.00	7295.0
63.00	6123.0
64.00	1182.0
65.00	1761.0
65.90	176.0
66.80	358.0
68.00	13874.0
69.00	14648.0
70.00	1021.0
72.10	779.0
73.00	6196.0
74.00	23800.0
75.00	69416.0
76.00	6191.0
77.00	882.0
77.90	748.0
78.90	5094.0
79.90	1545.0
80.90	5343.0
81.90	1326.0
83.00	116.0
85.70	174.0
87.00	6249.0
87.90	6272.0
90.90	446.0
92.00	3784.0
93.00	6009.0
94.00	15672.0
95.00	134336.0
96.00	8861.0
97.00	209.0
103.90	615.0
105.00	130.0
105.80	603.0
107.00	166.0
110.90	103.0
114.90	132.0
115.90	507.0
116.90	1061.0
117.80	533.0
119.00	861.0
127.80	404.0
128.00	407.0
128.90	267.0
129.90	487.0
131.00	244.0
134.90	223.0
136.90	272.0
140.90	1203.0
141.80	170.0
142.90	2148.0
143.90	149.0
144.90	792.0
145.90	221.0
147.90	301.0
149.90	159.0
154.90	266.0
156.90	250.0
158.70	131.0
161.00	114.0
171.00	288.0
172.00	1884.0
173.10	1524.0
174.00	98536.0
175.00	7518.0
175.90	93928.0
176.90	6345.0
177.90	231.0

Instrument :
MSVOA_U
ClientSampleId :
BFB183