

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122223\
 Data File : VU057220.D
 Acq On : 23 Dec 2023 04:15
 Operator : MD/SY
 Sample : 05979-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGR51

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU057220.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	86	95	108	rBV	93337	106349	14.97%	1.851%
2	1.911	185	193	206	rBV	82601	113695	16.00%	1.979%
3	2.564	383	396	412	rBV	156819	252256	35.50%	4.391%
4	3.175	575	586	602	rBV	5312	12327	1.73%	0.215%
5	4.625	1023	1037	1070	rBV	92694	258347	36.36%	4.497%
6	5.056	1154	1171	1209	rVB2	152222	357372	50.30%	6.221%
7	5.718	1356	1377	1409	rBV2	274572	710547	100.00%	12.369%
8	6.242	1528	1540	1561	rBV	215228	421123	59.27%	7.331%
9	6.682	1663	1677	1704	rBV	167295	336484	47.36%	5.858%
10	7.560	1937	1950	1974	rBV	77895	140007	19.70%	2.437%
11	7.891	2039	2053	2072	rBV	302998	545505	76.77%	9.496%
12	8.174	2130	2141	2164	rBV3	46454	82836	11.66%	1.442%
13	8.467	2223	2232	2244	rBV3	9615	17057	2.40%	0.297%
14	8.628	2271	2282	2322	rBV2	338289	662067	93.18%	11.526%
15	9.412	2513	2526	2545	rBV	309920	533671	75.11%	9.290%
16	10.750	2930	2942	2958	rBV2	122510	200641	28.24%	3.493%
17	10.885	2975	2984	2995	rBV	17306	26454	3.72%	0.461%
18	11.808	3259	3271	3298	rBV	281613	464067	65.31%	8.079%
19	12.187	3375	3389	3406	rBV	287047	473944	66.70%	8.251%
20	14.570	4118	4130	4147	rBV	12822	20303	2.86%	0.353%
21	16.881	4842	4849	4856	rVB4	7166	9299	1.31%	0.162%




Sum of corrected areas: 5744351

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122223\
Data File : VU057220.D
Acq On : 23 Dec 2023 04:15
Operator : MD/SY
Sample : 05979-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGR51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

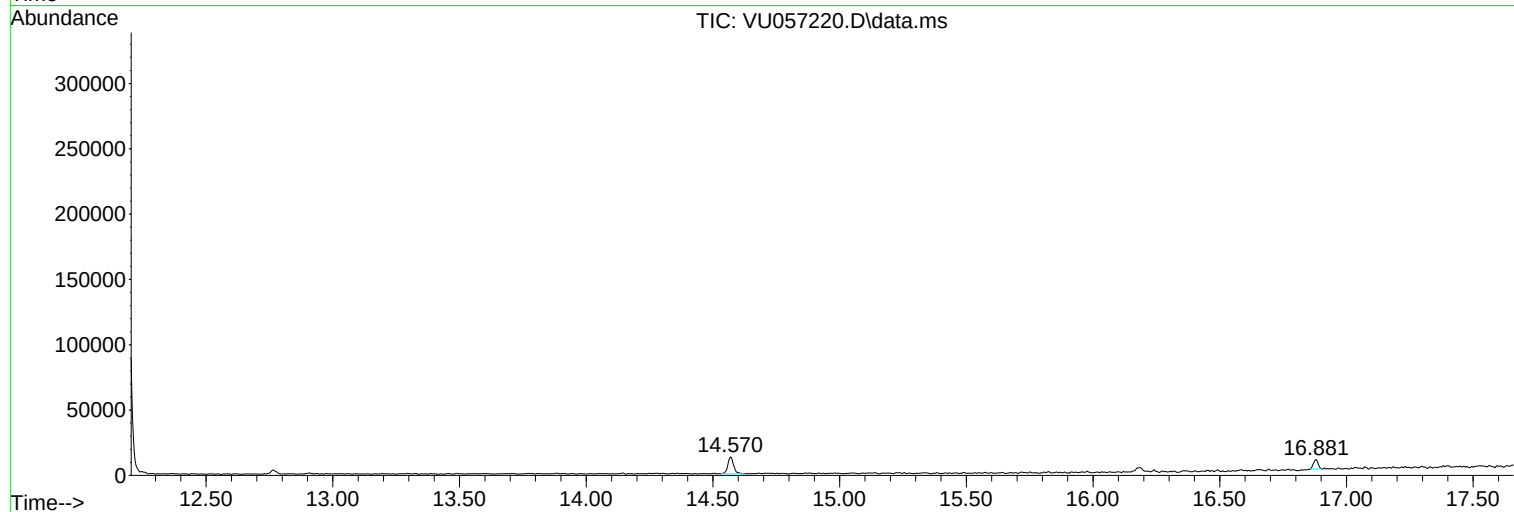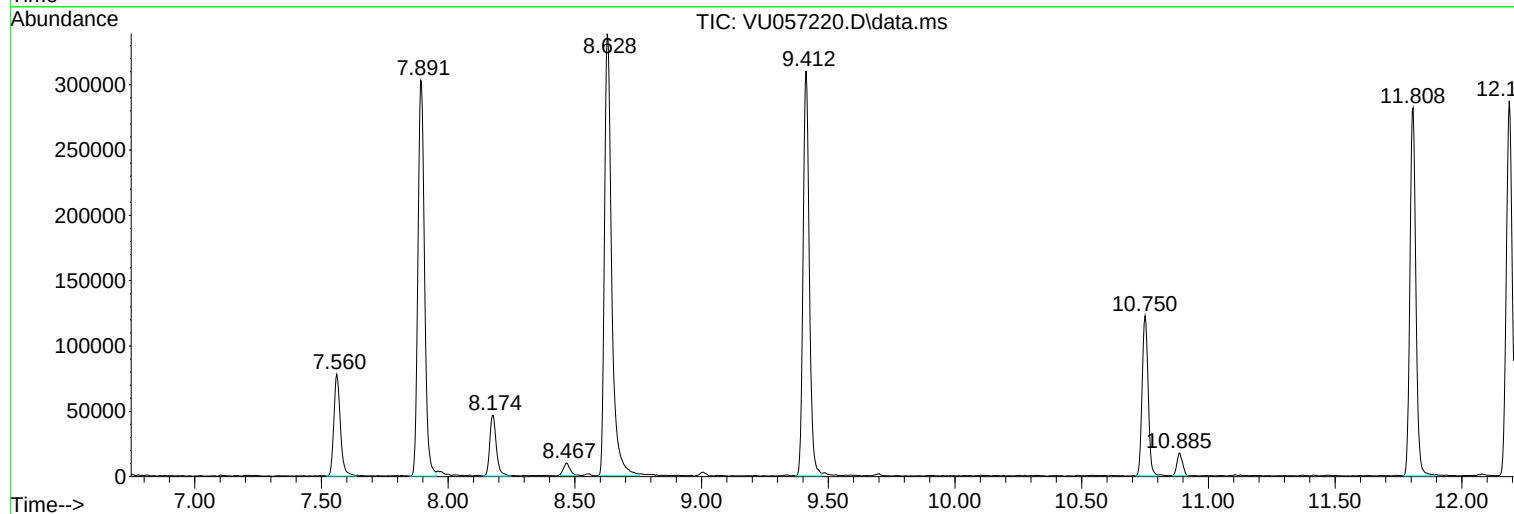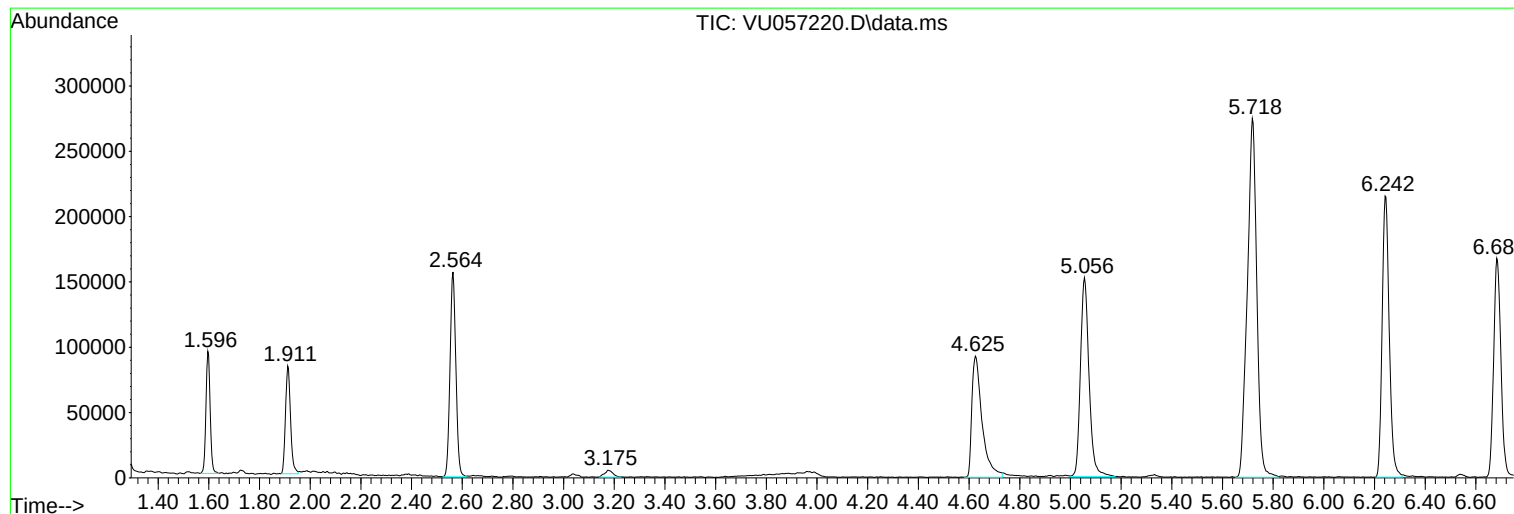

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122223\
Data File : VU057220.D
Acq On : 23 Dec 2023 04:15
Operator : MD/SY
Sample : 05979-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGR51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122223\
Data File : VU057220.D
Acq On : 23 Dec 2023 04:15
Operator : MD/SY
Sample : 05979-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGR51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc