

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122223\
 Data File : VU057222.D
 Acq On : 23 Dec 2023 05:03
 Operator : MD/SY
 Sample : 05979-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGR53

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU057222.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	107	rVB	93413	108007	14.96%	1.914%
2	1.911	184	193	206	rBV	81407	113024	15.65%	2.003%
3	2.563	384	396	412	rBV	152631	250780	34.72%	4.445%
4	3.181	573	588	600	rBV2	5434	10953	1.52%	0.194%
5	4.621	1022	1036	1064	rBV	93156	248586	34.42%	4.406%
6	5.055	1155	1171	1194	rBV	153125	339109	46.96%	6.010%
7	5.718	1351	1377	1401	rBV2	275234	722197	100.00%	12.800%
8	6.242	1525	1540	1559	rBV	207531	400184	55.41%	7.093%
9	6.685	1663	1678	1698	rBV	173258	341218	47.25%	6.048%
10	7.560	1937	1950	1965	rBV2	77099	140705	19.48%	2.494%
11	7.894	2037	2054	2071	rBV	314836	558347	77.31%	9.896%
12	8.174	2131	2141	2167	rVB2	46504	85420	11.83%	1.514%
13	8.467	2222	2232	2242	rBV4	5320	9624	1.33%	0.171%
14	8.627	2271	2282	2313	rBV	343713	653939	90.55%	11.590%
15	9.412	2511	2526	2549	rBV	295266	510389	70.67%	9.046%
16	10.750	2927	2942	2957	rBV2	118936	197255	27.31%	3.496%
17	10.885	2974	2984	2996	rVB2	8844	14076	1.95%	0.249%
18	11.807	3259	3271	3291	rBV	271019	445399	61.67%	7.894%
19	12.187	3376	3389	3412	rBV	290399	477824	66.16%	8.469%
20	14.569	4120	4130	4140	rBV2	8934	15086	2.09%	0.267%




Sum of corrected areas: 5642122

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122223\
Data File : VU057222.D
Acq On : 23 Dec 2023 05:03
Operator : MD/SY
Sample : 05979-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGR53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

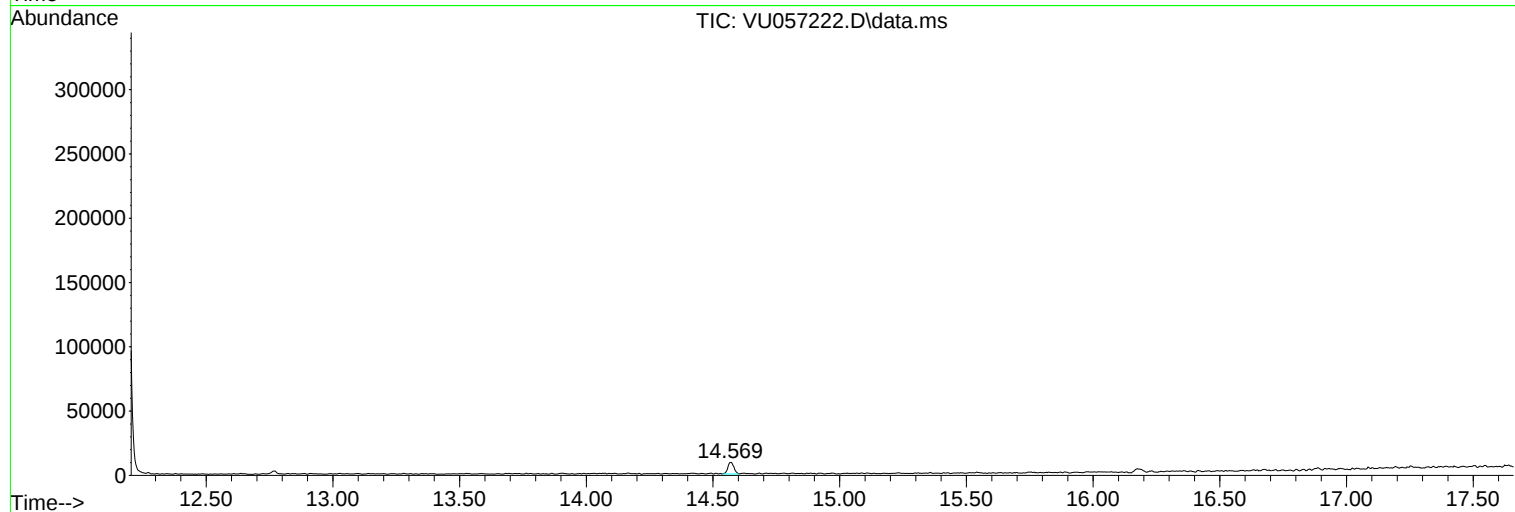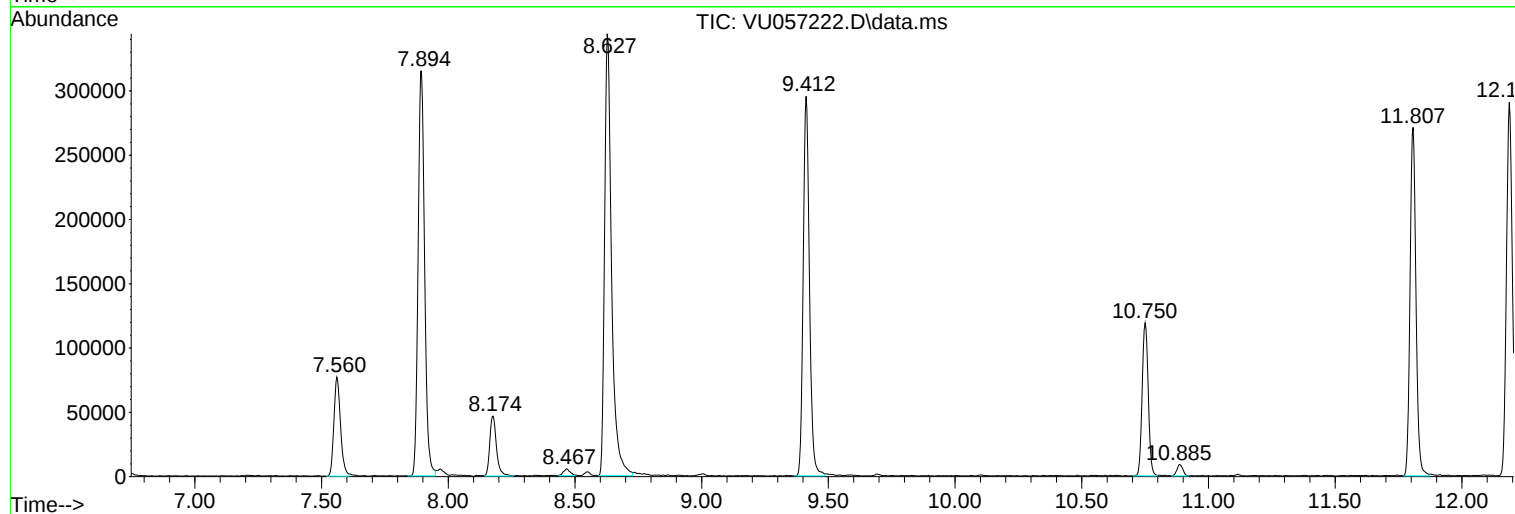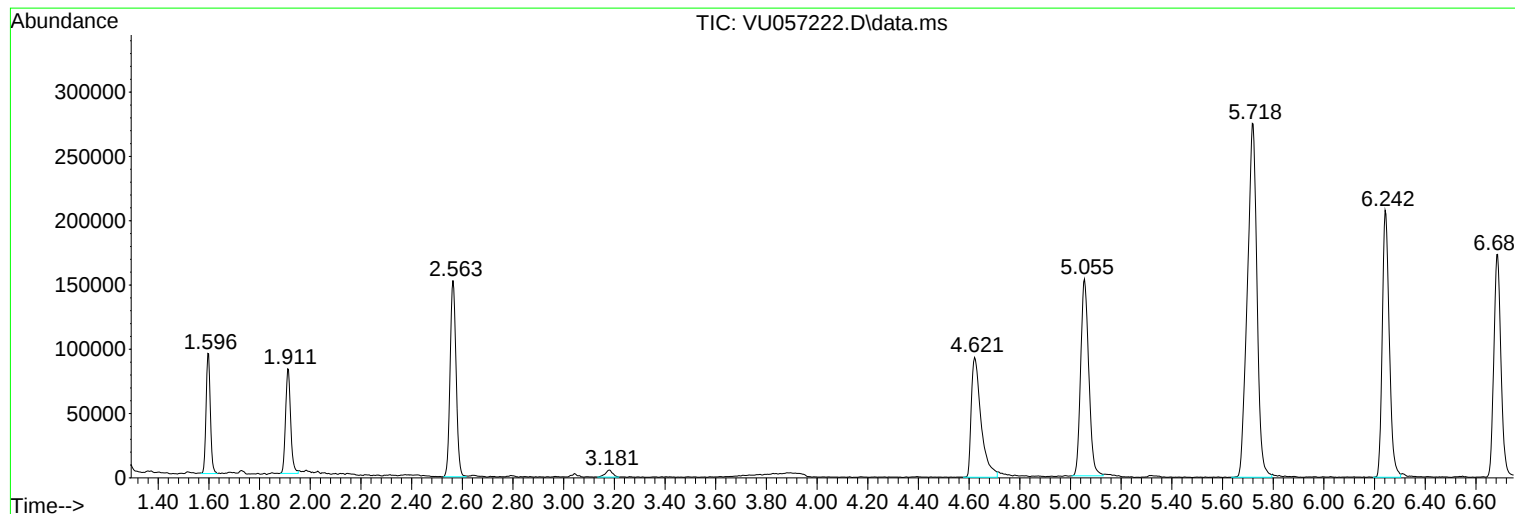

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122223\
Data File : VU057222.D
Acq On : 23 Dec 2023 05:03
Operator : MD/SY
Sample : 05979-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGR53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122223\
Data File : VU057222.D
Acq On : 23 Dec 2023 05:03
Operator : MD/SY
Sample : 05979-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGR53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc