

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122223\
 Data File : VU057228.D
 Acq On : 23 Dec 2023 07:29
 Operator : MD/SY
 Sample : 05979-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BGRS6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU057228.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	108	rVB	93933	110637	15.05%	1.930%
2	1.911	184	193	208	rBV	83106	116070	15.79%	2.024%
3	2.563	384	396	411	rBV	159933	260651	35.45%	4.546%
4	3.177	576	587	600	rVB2	4468	8489	1.15%	0.148%
5	4.621	1022	1036	1068	rBV	95433	259835	35.34%	4.532%
6	5.055	1155	1171	1197	rBV	154005	349330	47.51%	6.093%
7	5.721	1357	1378	1402	rBV2	280372	735279	100.00%	12.824%
8	6.245	1527	1541	1560	rBV	199605	388485	52.84%	6.776%
9	6.682	1662	1677	1695	rBV2	176422	351364	47.79%	6.128%
10	7.560	1939	1950	1968	rBV2	79543	142651	19.40%	2.488%
11	7.894	2041	2054	2072	rBV	317313	565832	76.95%	9.869%
12	7.965	2073	2076	2094	rVB3	4664	8224	1.12%	0.143%
13	8.177	2131	2142	2159	rBV	48974	85548	11.63%	1.492%
14	8.470	2220	2233	2244	rBV5	3819	8239	1.12%	0.144%
15	8.627	2271	2282	2311	rBV2	356177	691846	94.09%	12.067%
16	9.412	2510	2526	2555	rBV	284578	500812	68.11%	8.735%
17	10.750	2930	2942	2960	rBV	125833	205288	27.92%	3.581%
18	10.888	2975	2985	2995	rBV2	7389	11330	1.54%	0.198%
19	11.807	3260	3271	3295	rBV	261803	429338	58.39%	7.488%
20	12.187	3374	3389	3411	rBV2	299386	491619	66.86%	8.575%
21	14.569	4120	4130	4140	rBV2	8064	12579	1.71%	0.219%




Sum of corrected areas: 5733446

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122223\
Data File : VU057228.D
Acq On : 23 Dec 2023 07:29
Operator : MD/SY
Sample : 05979-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGRS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

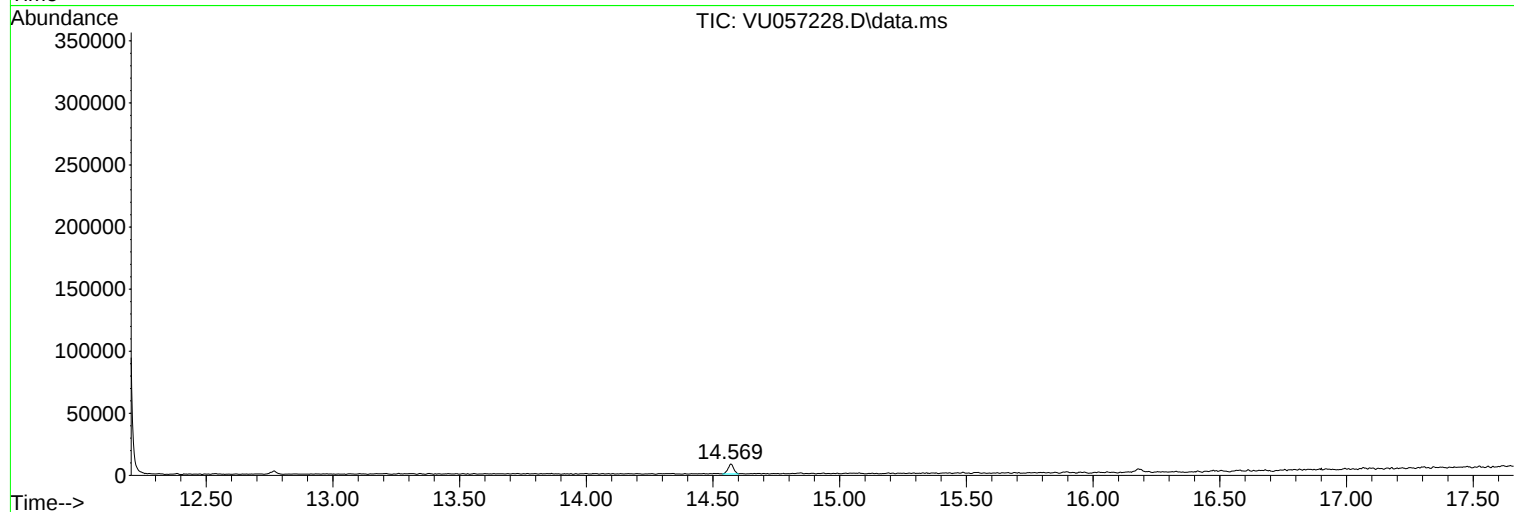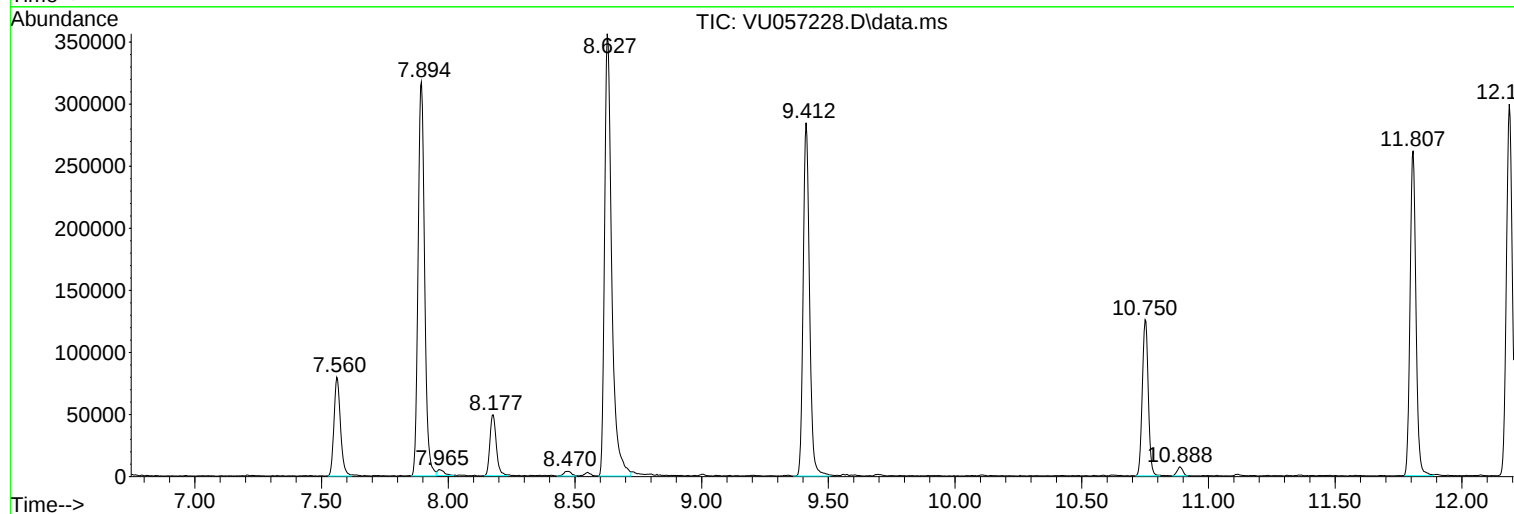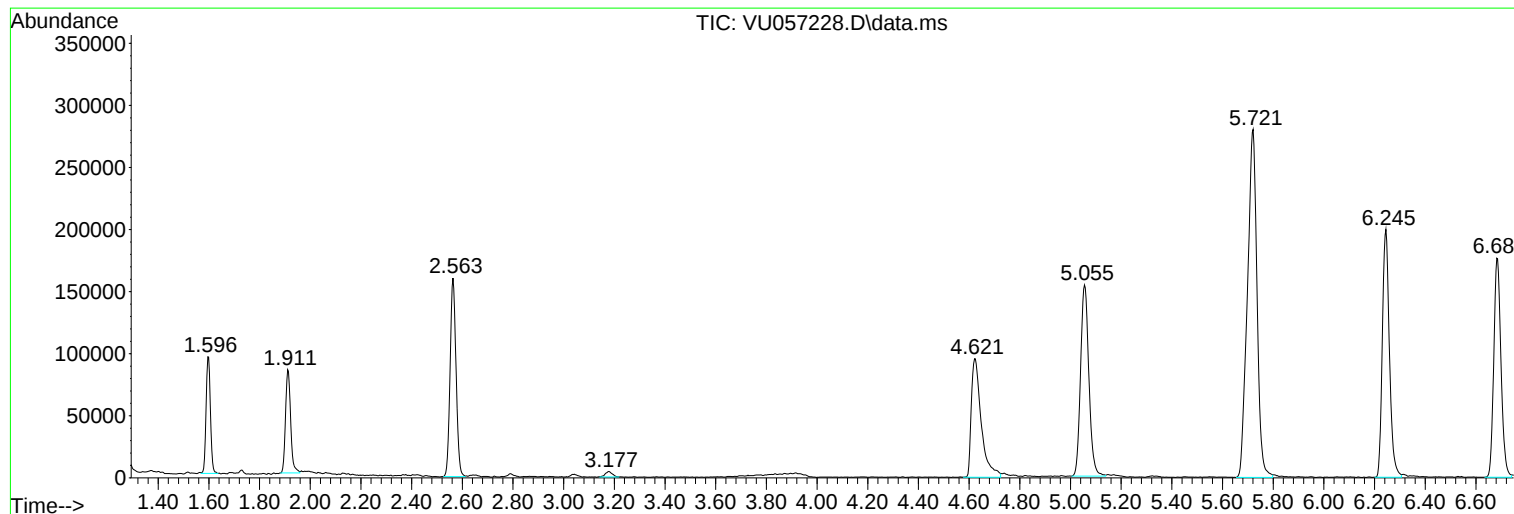

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122223\
Data File : VU057228.D
Acq On : 23 Dec 2023 07:29
Operator : MD/SY
Sample : 05979-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGRS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122223\
Data File : VU057228.D
Acq On : 23 Dec 2023 07:29
Operator : MD/SY
Sample : 05979-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BGRS6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc