
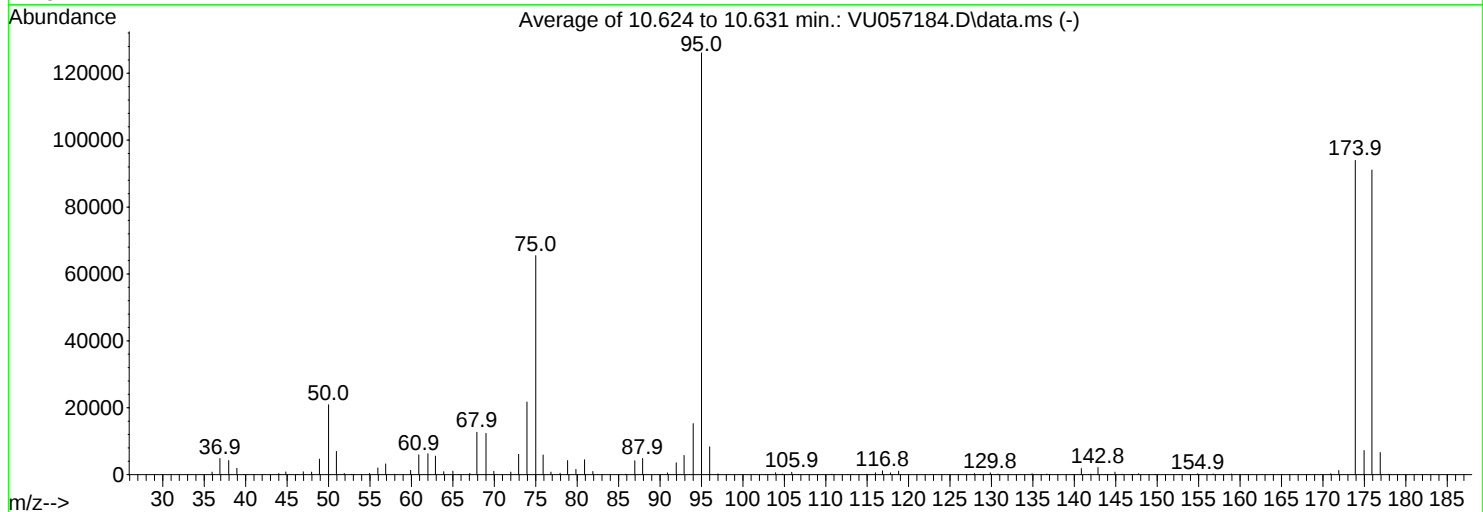


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122223\
Data File : VU057184.D
Acq On : 22 Dec 2023 12:24
Operator : MD/SY
Sample : BFB100
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB100

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Dec 23 00:27:07 2023

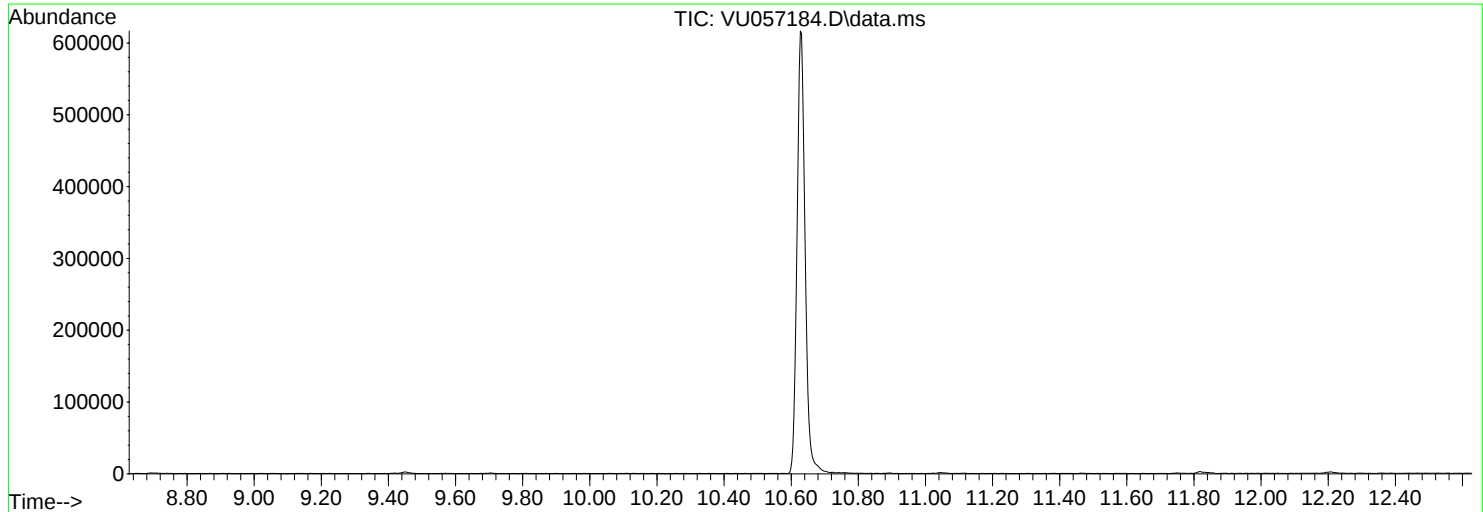

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.6	20891	PASS
75	95	30	80	51.9	65475	PASS
95	95	100	100	100.0	126096	PASS
96	95	5	9	6.6	8327	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.5	93952	PASS
175	174	5	9	7.7	7230	PASS
176	174	95	101	96.9	91064	PASS
177	176	5	9	7.2	6601	PASS

m/z	Abundance
39.80	285.0
44.00	295.0

Instrument :
MSVOA_U
ClientSampleId :
BFB100

m/z	Abundance
36.00	797.0
36.90	4602.0
38.00	4088.0
39.00	1820.0
39.90	282.0
44.00	555.0
44.80	822.0
46.20	146.0
46.90	881.0
47.90	815.0
48.90	4403.0
50.00	19888.0
50.90	6678.0
51.90	499.0
52.80	214.0
55.00	436.0
56.00	1986.0
56.90	3021.0
57.90	171.0
59.90	1342.0
60.90	5779.0
62.00	6047.0
62.90	5301.0
63.90	892.0
65.00	942.0
67.10	388.0
67.90	12119.0
69.00	12129.0
70.00	962.0
72.00	866.0
72.90	5689.0
74.00	20248.0
75.00	62512.0
75.90	5937.0
76.80	865.0
77.90	503.0
78.90	4164.0
79.90	1404.0
80.90	4140.0
81.90	846.0
85.80	149.0
87.00	4098.0
87.90	4601.0
90.90	457.0
91.90	3168.0
92.90	5211.0
94.00	14271.0
95.00	118688.0
96.00	7970.0
97.00	214.0
103.90	549.0
104.80	149.0
105.90	708.0
106.70	111.0
110.00	102.0
110.70	121.0
114.90	194.0
116.00	546.0
116.90	1130.0
117.80	556.0
118.80	984.0
128.00	346.0
128.70	179.0
129.80	586.0
130.80	195.0
134.90	337.0
136.70	270.0
140.80	1679.0
142.90	2115.0
143.80	125.0
144.90	753.0
145.70	153.0
146.90	110.0
147.80	349.0
154.90	232.0
156.80	213.0
159.00	120.0
170.90	298.0
171.90	1143.0
173.90	85888.0
174.90	6523.0
175.90	84672.0
176.90	6351.0
178.00	199.0

Instrument :
MSVOA_U
ClientSampleId :
BFB100

m/z	Abundance
36.00	766.0
36.90	5016.0
38.00	4314.0
39.00	1939.0
39.80	325.0
44.00	646.0
44.90	820.0
46.20	128.0
46.90	832.0
48.00	743.0
48.90	4763.0
50.00	21664.0
51.00	7213.0
51.90	403.0
52.80	148.0
54.90	417.0
56.00	2108.0
56.90	3293.0
57.90	170.0
59.90	1320.0
60.90	6086.0
62.00	6578.0
62.90	5829.0
63.90	1010.0
65.00	1088.0
67.00	445.0
67.90	13148.0
69.00	12633.0
70.00	1022.0
72.00	809.0
73.00	6261.0
73.90	22328.0
75.00	67256.0
75.90	6175.0
76.80	743.0
77.90	471.0
78.80	4384.0
79.80	1647.0
80.90	4586.0
81.90	989.0
82.50	119.0
85.80	152.0
87.00	4291.0
87.90	5069.0
90.90	528.0
91.90	3616.0
92.90	5843.0
94.00	15832.0
95.00	130224.0
96.00	8445.0
97.00	233.0
102.80	115.0
104.00	570.0
104.70	213.0
105.90	737.0
109.90	114.0
110.70	162.0
112.60	100.0
115.00	179.0
116.00	608.0
116.90	1194.0
117.80	540.0
118.80	1114.0
128.00	391.0
128.70	148.0
129.20	165.0
129.80	526.0
130.80	193.0
134.90	323.0
136.70	283.0
140.90	1926.0
141.70	195.0
142.00	210.0
142.90	2247.0
143.80	108.0
144.90	808.0
145.70	149.0
147.80	317.0
149.80	143.0
154.90	289.0
156.70	264.0
158.90	200.0
170.90	322.0
171.90	1268.0
173.90	97176.0
175.00	7568.0
175.90	93912.0
176.90	6888.0
177.90	152.0

Instrument :
MSVOA_U
ClientSampleId :
BFB100

m/z	Abundance
35.90	728.0
36.90	4892.0
37.90	4254.0
38.90	2011.0
39.80	365.0
44.00	755.0
44.90	772.0
47.00	810.0
48.00	680.0
48.90	4709.0
50.00	21120.0
51.00	7005.0
51.90	294.0
53.10	157.0
54.90	393.0
55.90	1983.0
56.90	3314.0
58.00	133.0
59.90	1238.0
60.90	5956.0
62.00	6228.0
62.90	5568.0
63.90	883.0
65.00	1131.0
65.70	114.0
67.00	388.0
67.90	12767.0
69.00	12203.0
69.90	999.0
72.00	622.0
73.00	6227.0
73.90	22536.0
75.00	66656.0
75.90	5601.0
76.90	674.0
78.00	351.0
78.80	4047.0
79.80	1639.0
80.90	4701.0
81.90	1084.0
85.90	131.0
86.90	4119.0
87.90	4903.0
90.90	573.0
92.00	3872.0
92.90	6163.0
94.00	15738.0
95.00	129376.0
96.00	8567.0
97.00	278.0
102.70	141.0
103.90	545.0
104.70	279.0
105.90	740.0
109.90	138.0
110.80	145.0
112.70	130.0
114.90	121.0
116.00	549.0
116.80	1144.0
117.80	505.0
118.80	1102.0
127.90	349.0
129.00	143.0
129.90	451.0
130.80	152.0
134.90	265.0
137.00	300.0
140.90	1869.0
141.90	238.0
142.80	2073.0
143.80	101.0
144.90	706.0
145.80	198.0
147.70	279.0
149.70	160.0
152.70	103.0
154.90	317.0
156.70	287.0
158.90	220.0
160.70	110.0
171.00	290.0
171.90	1326.0
173.90	98792.0
175.00	7599.0
175.90	94608.0
176.90	6563.0
177.90	104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB100