

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U122320\
 Data File : VU041773.D
 Acq On : 23 Dec 2020 11:34
 Operator : SY/MD
 Sample : L5161-11DL 2X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB236DL

Quant Time: Dec 24 01:27:48 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 24 01:08:18 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	146820	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	142010	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	62031	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	43717	3.81	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.20%
7) Chloroethane-d5	1.92	69	44666	5.03	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	100.60%
11) 1,1-Dichloroethene-d2	2.58	63	65862	3.12	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.40%
20) 2-Butanone-d5	4.66	46	153180	46.46	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	92.92%
24) Chloroform-d	5.08	84	89277	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.80%
26) 1,2-Dichloroethane-d4	5.72	65	51598	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.60%
32) Benzene-d6	5.74	84	173238	4.26	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.20%
36) 1,2-Dichloropropane-d6	6.70	67	55597	4.36	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.20%
41) Toluene-d8	7.90	98	138559	3.78	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	75.60%
43) trans-1,3-Dichloropropene-	8.19	79	21854	3.81	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.20%
46) 2-Hexanone-d5	8.64	63	137847	43.99	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.98%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	52704	4.55	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.00%
64) 1,2-Dichlorobenzene-d4	12.19	152	54043	4.90	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.00%


Target Compounds					Ovalue
31) Carbon tetrachloride	5.54	117	99861	7.082 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU122320\
Data File : VU041773.D
Acq On : 23 Dec 2020 11:34
Operator : SY/MD
Sample : L5161-11DL 2X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB236DL

Quant Time: Dec 24 01:27:48 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 24 01:08:18 2020
Response via : Initial Calibration

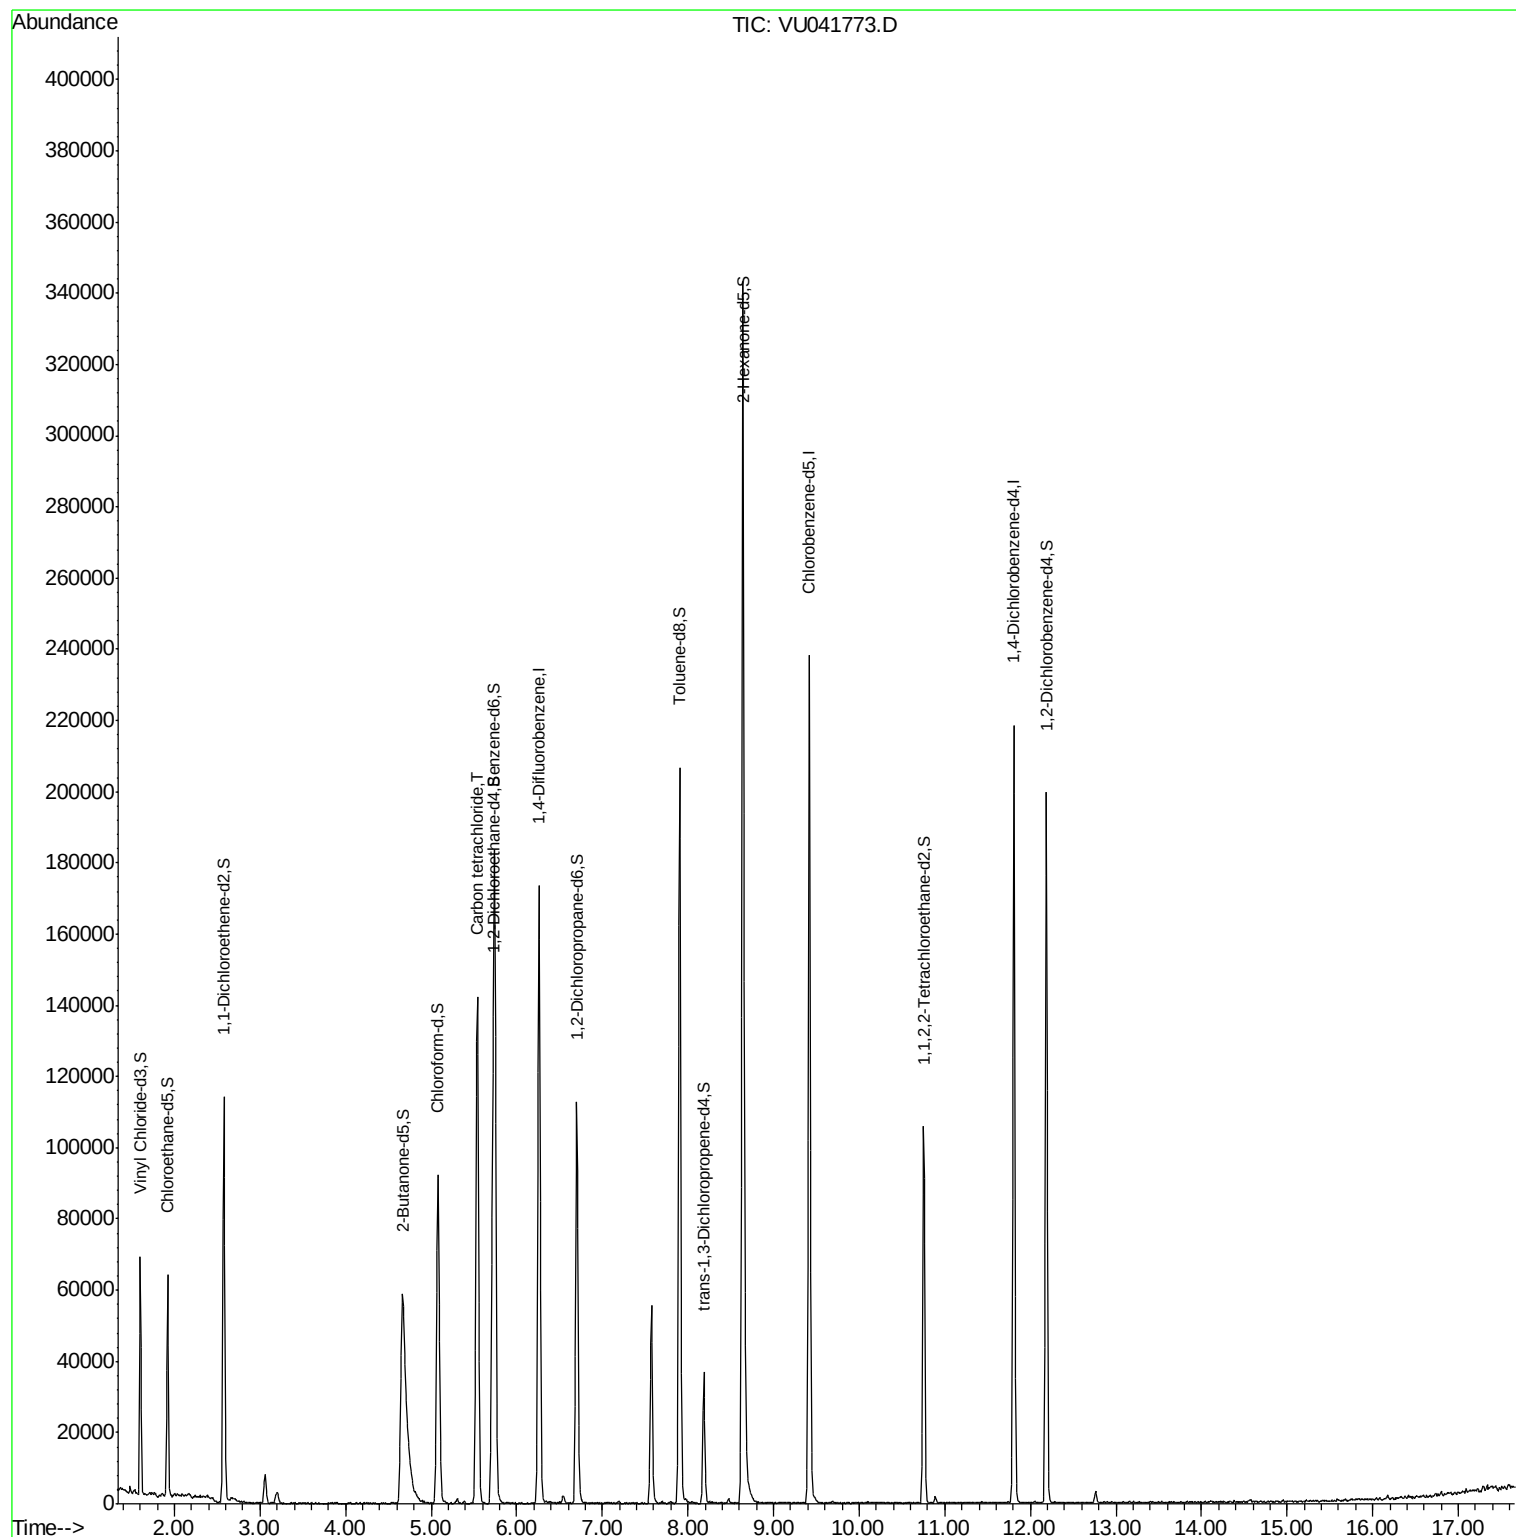

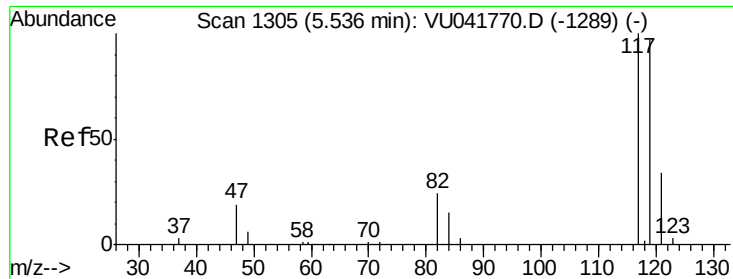

#31

Carbon tetrachloride

Concen: 7.082 ug/L

RT: 5.54 min Scan# 1306

Delta R.T. 0.00 min

Lab File: VU041773.D

Acq: 23 Dec 2020 11:34

Instrument :

MSVOA_U

ClientSampleId :

GB236DL

Tot Ion:117 Resp: 99861

Ion Ratio Lower Upper

117 100

119 96.4 76.2 114.2

