

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U122320\
 Data File : VU041782.D
 Acq On : 23 Dec 2020 15:03
 Operator : SY/MD
 Sample : L5161-19DL 50X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB244DL

Quant Time: Dec 24 03:27:00 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Dec 24 01:08:18 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	132097	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	116057	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	54668	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	39198	3.80	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	76.00%
7) Chloroethane-d5	1.92	69	41837	5.23	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.60%
11) 1,1-Dichloroethene-d2	2.58	63	57961	3.05	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.00%
20) 2-Butanone-d5	4.66	46	186303	62.80	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	125.60%
24) Chloroform-d	5.08	84	92571	5.23	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	104.60%
26) 1,2-Dichloroethane-d4	5.72	65	55477	5.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	110.60%
32) Benzene-d6	5.74	84	179522	5.40	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	108.00%
36) 1,2-Dichloropropane-d6	6.70	67	57746	5.54	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	110.80%
41) Toluene-d8	7.90	98	124206	4.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.80%
43) trans-1,3-Dichloropropene-	8.19	79	22002	4.70	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	94.00%
46) 2-Hexanone-d5	8.64	63	136856	53.44	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	106.88%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	54116	5.72	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	114.40%
64) 1,2-Dichlorobenzene-d4	12.19	152	51672	5.32	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.40%


Target Compounds					Ovalue
31) Carbon tetrachloride	5.54	117	114076	9.899 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU122320\
Data File : VU041782.D
Acq On : 23 Dec 2020 15:03
Operator : SY/MD
Sample : L5161-19DL 50X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB244DL

Quant Time: Dec 24 03:27:00 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Dec 24 01:08:18 2020
Response via : Initial Calibration

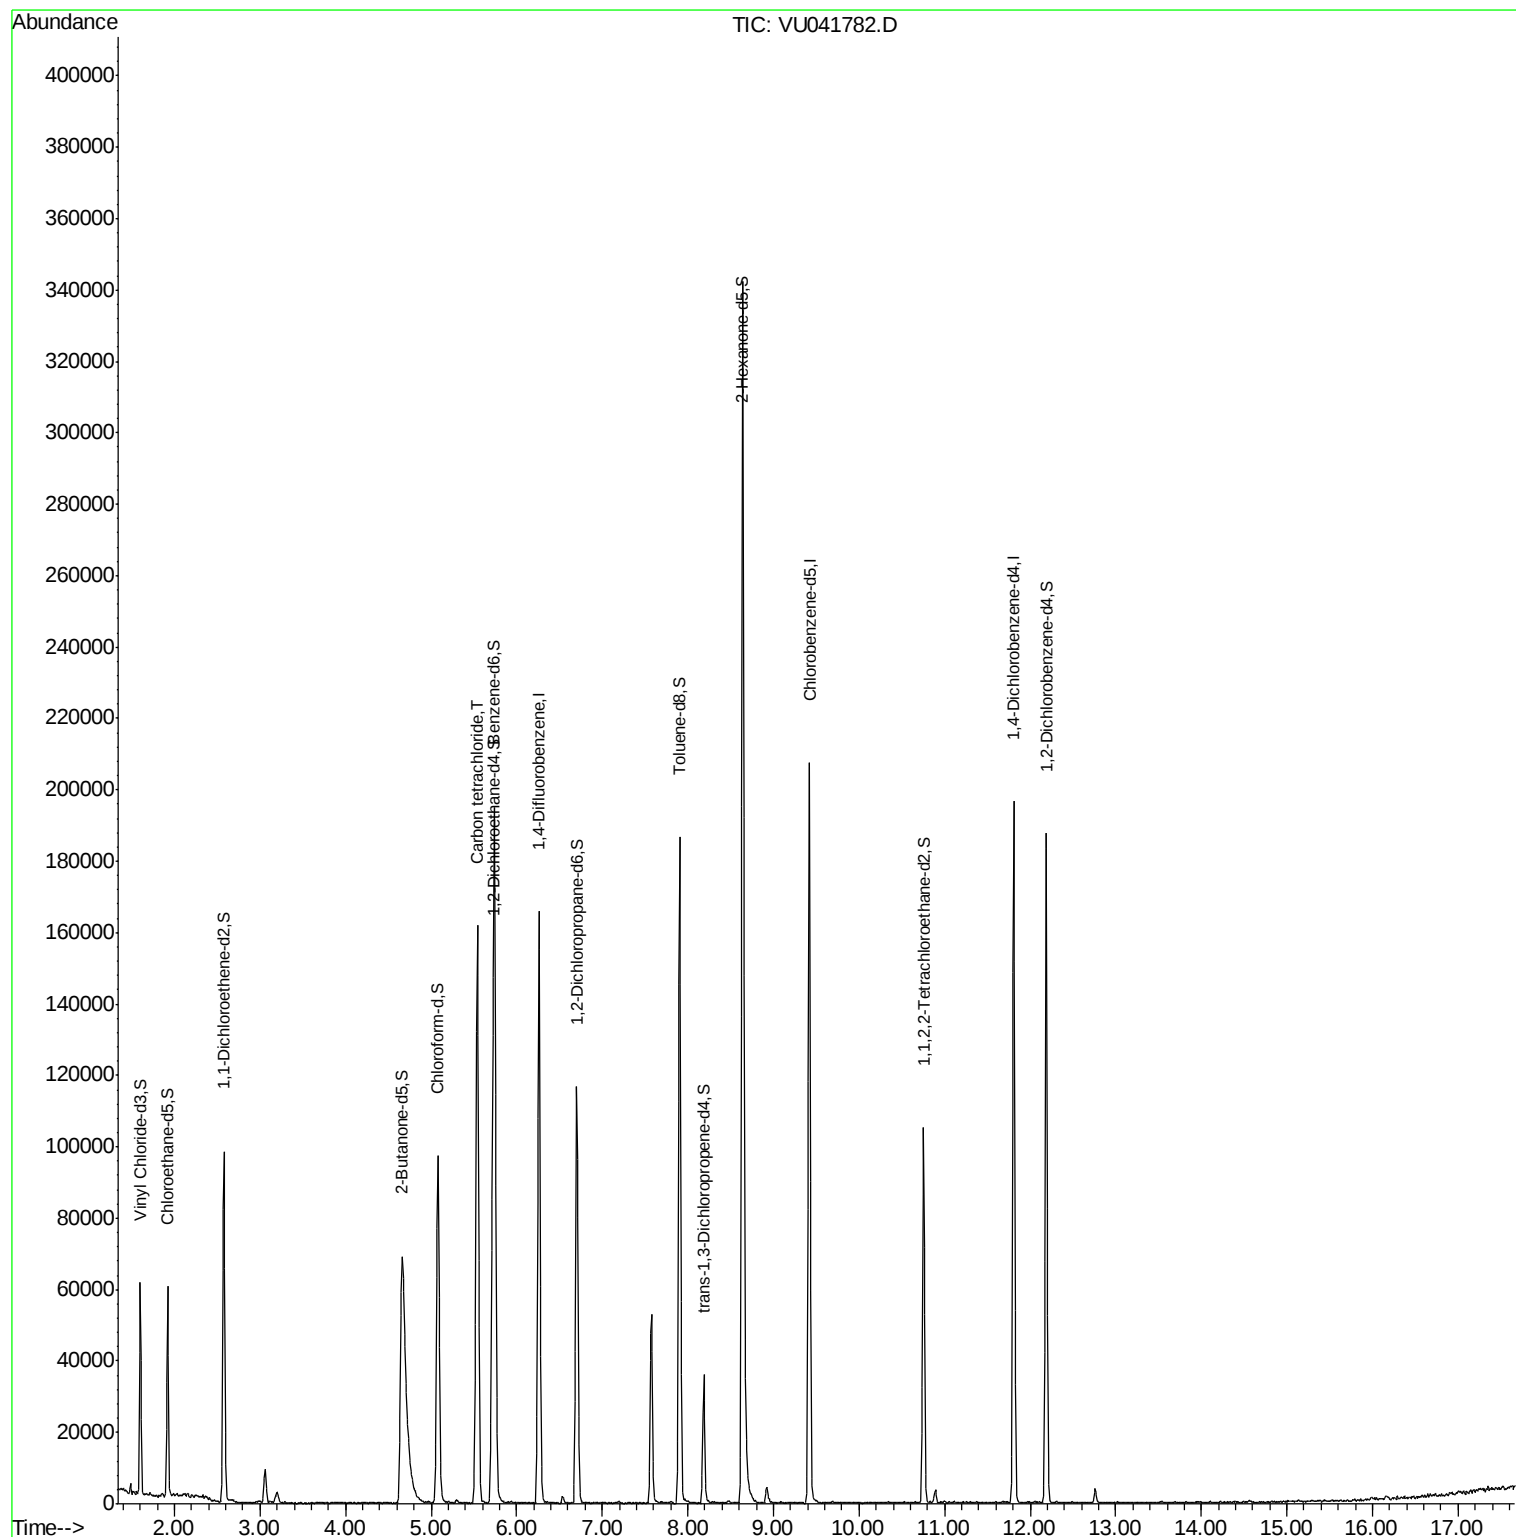

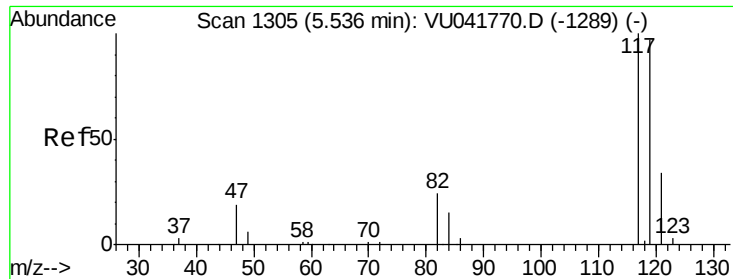

#31

Carbon tetrachloride

Concen: 9.899 ug/L

RT: 5.54 min Scan# 1306

Delta R.T. 0.00 min

Lab File: VU041782.D

Acq: 23 Dec 2020 15:03

Instrument :

MSVOA_U

ClientSampleId :

GB244DL

Tot Ion:117 Resp: 114076

Ion Ratio Lower Upper

117 100

119 96.9 76.2 114.2

