


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU122320\
 Data File : VU041769.D
 Acq On : 23 Dec 2020 08:44
 Operator : SY/MD
 Sample : BFB29
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB29

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Dec 24 01:08:18 2020

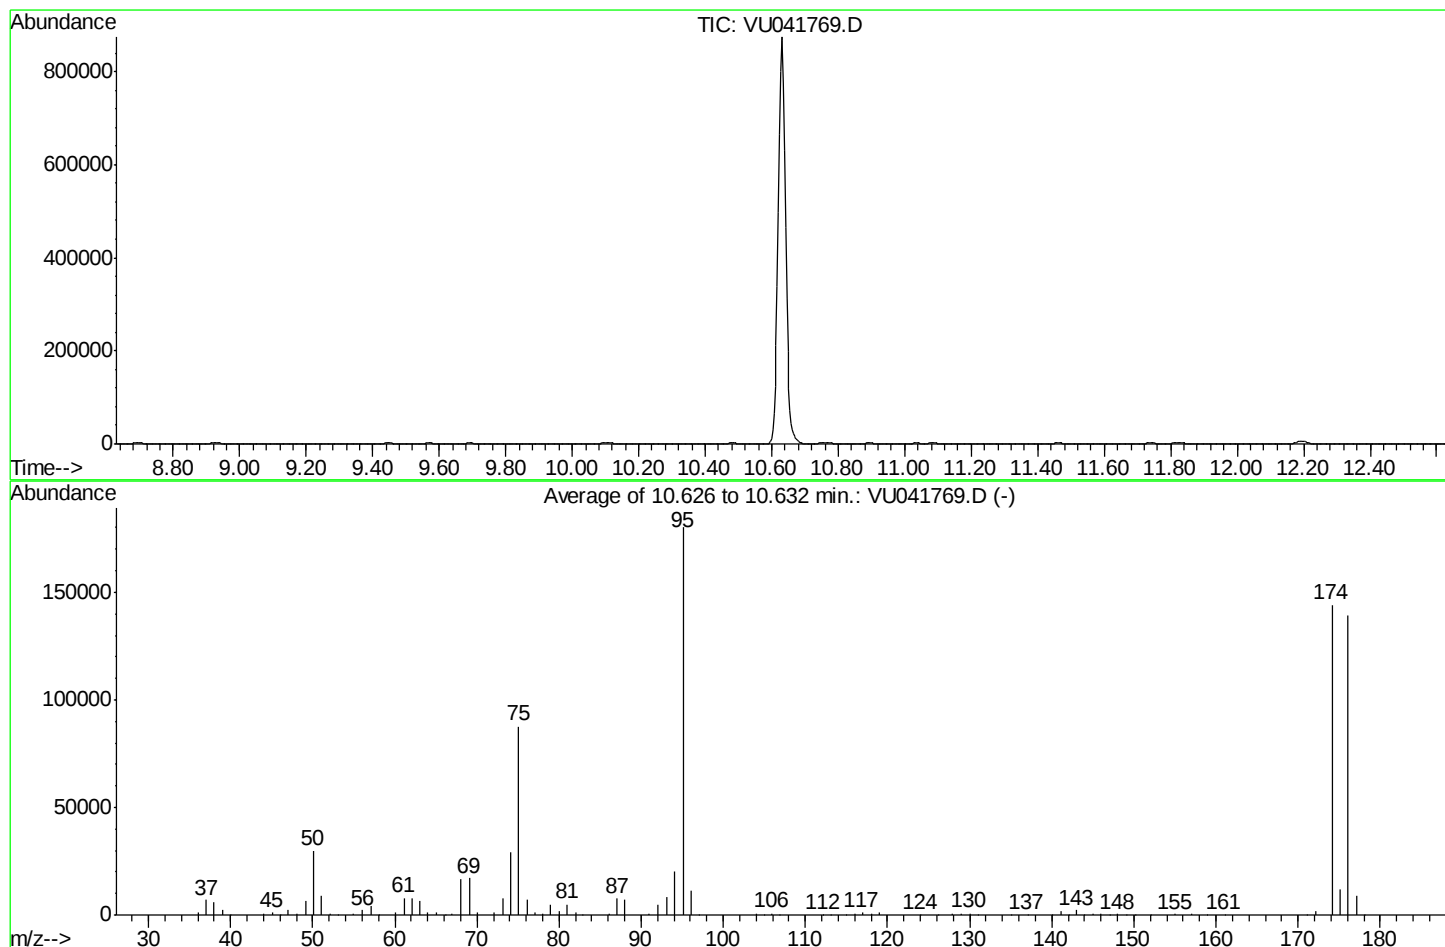

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2874

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.5	29765	PASS
75	95	30	80	48.7	87669	PASS
95	95	100	100	100.0	180181	PASS
96	95	5	9	6.3	11355	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.9	144042	PASS
175	174	5	9	8.1	11685	PASS
176	174	95	101	96.8	139426	PASS
177	176	5	9	6.6	9189	PASS

m/z	Abundance
36.10	1167.0
37.10	6719.0
38.00	5471.0
39.10	2109.0
40.00	200.0
44.10	884.0
45.10	921.0
46.00	108.0
47.00	2089.0
48.00	797.0
49.10	6031.0
50.10	28600.0
51.10	8630.0
52.10	449.0
53.00	130.0
55.00	437.0
56.10	2288.0
57.00	3938.0
58.00	165.0
60.10	1386.0
61.10	7530.0
62.10	7301.0
63.10	6587.0
64.00	914.0
65.10	1488.0
66.20	128.0
67.00	436.0
68.10	15994.0
69.10	16259.0
70.10	1241.0
72.10	896.0
73.10	7629.0
74.10	28104.0
75.10	83472.0
76.10	6899.0
77.10	787.0
78.00	647.0
79.00	4732.0
80.00	1550.0
81.00	4583.0
82.00	1028.0
86.00	332.0
87.10	7531.0
88.00	7348.0
91.00	719.0
92.10	4674.0
93.10	7864.0
94.10	19448.0
95.10	170176.0
96.10	11178.0
97.00	288.0
104.00	755.0
105.00	237.0
106.00	757.0
106.90	109.0
115.00	238.0
116.00	660.0
116.90	1048.0
118.00	536.0
119.00	1097.0
124.00	135.0
126.10	141.0
127.90	535.0
128.90	356.0
130.00	559.0
131.00	191.0
135.00	270.0
137.00	293.0
140.10	111.0
141.10	1529.0
142.00	162.0
143.00	2093.0
144.00	117.0
145.00	646.0
146.00	309.0
148.10	337.0
150.10	217.0
152.00	186.0
155.00	294.0
157.00	357.0
159.00	151.0
161.00	150.0
171.10	249.0
172.10	1906.0
174.10	134208.0
175.10	10744.0
176.10	129896.0
177.10	8167.0
178.10	242.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

m/z	Abundance
36.10	1127.0
37.10	7418.0
38.00	5867.0
39.00	2454.0
40.00	173.0
44.10	895.0
45.10	1045.0
47.10	2370.0
48.00	847.0
49.10	6473.0
50.10	30736.0
51.10	9295.0
52.10	474.0
53.00	147.0
55.00	385.0
56.10	2415.0
57.00	4182.0
58.00	147.0
60.00	1328.0
61.10	8255.0
62.10	7928.0
63.10	6896.0
64.00	1017.0
65.10	1485.0
66.20	105.0
67.00	555.0
68.10	17160.0
69.10	17760.0
70.10	1258.0
72.10	931.0
73.10	8181.0
74.10	30336.0
75.10	90624.0
76.10	7587.0
77.10	880.0
78.00	829.0
79.00	4599.0
80.00	1678.0
81.00	4974.0
82.00	1186.0
82.90	114.0
86.10	357.0
87.10	7949.0
88.00	7732.0
91.00	743.0
92.10	5119.0
93.10	8509.0
94.10	20896.0
95.10	185920.0
96.10	11656.0
97.00	291.0
104.00	734.0
105.00	255.0
105.90	844.0
106.90	151.0
112.20	106.0
113.00	129.0
115.00	281.0
116.00	829.0
116.90	1175.0
118.00	549.0
119.00	1116.0
124.00	146.0
126.10	122.0
127.90	532.0
128.90	431.0
130.00	627.0
131.00	172.0
135.00	313.0
137.00	309.0
140.00	128.0
141.10	1619.0
142.00	211.0
143.10	2302.0
143.90	147.0
145.10	694.0
146.00	373.0
148.00	478.0
149.10	121.0
150.10	189.0
152.00	169.0
155.00	357.0
157.00	384.0
158.90	221.0
161.00	143.0
171.10	269.0
172.10	2013.0
174.10	148160.0
175.10	12116.0
176.10	144192.0
177.10	9488.0
178.00	268.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

m/z	Abundance
36.10	1055.0
37.00	7156.0
38.00	5733.0
39.00	2538.0
40.00	159.0
44.10	850.0
45.10	1162.0
47.10	2222.0
48.00	846.0
49.10	6346.0
50.10	29960.0
51.10	9007.0
52.10	404.0
53.00	152.0
55.00	279.0
56.10	2318.0
57.10	3942.0
58.10	129.0
60.00	1340.0
61.10	7970.0
62.10	8023.0
63.10	6558.0
64.00	1013.0
65.10	1387.0
67.00	585.0
68.10	16992.0
69.10	17240.0
70.00	1231.0
72.10	913.0
73.10	7948.0
74.10	29360.0
75.10	88912.0
76.10	7577.0
77.10	1089.0
78.10	943.0
79.00	4207.0
80.00	1595.0
81.00	4928.0
82.00	1251.0
82.90	122.0
86.10	384.0
87.10	7552.0
88.00	7162.0
91.00	654.0
92.10	5093.0
93.10	8184.0
94.10	20232.0
95.10	184448.0
96.10	11232.0
97.00	303.0
104.00	703.0
105.00	252.0
106.00	837.0
106.90	161.0
113.00	139.0
115.00	305.0
116.00	888.0
117.00	1148.0
118.00	505.0
119.00	1056.0
128.00	542.0
128.90	392.0
130.00	644.0
131.00	154.0
135.00	283.0
137.00	306.0
139.90	160.0
141.10	1581.0
142.10	246.0
143.10	2133.0
143.90	151.0
145.10	669.0
146.00	361.0
147.00	100.0
148.00	528.0
149.10	154.0
150.00	124.0
152.00	161.0
155.10	442.0
157.00	334.0
159.00	262.0
161.10	157.0
171.10	280.0
172.10	1914.0
174.10	149760.0
175.10	12197.0
176.10	144192.0
177.10	9912.0
178.00	301.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29

m/z	Abundance
43.90	201.0

Instrument :
MSVOA_U
ClientSampleId :
BFB29