




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122321\
Data File : VU046576.D
Acq On : 23 Dec 2021 19:25
Operator : SY/MD
Sample : M5175-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBBY5

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 12/24/2021
Supervised By :Semsettin Yesilyurt 01/02/2022

Quant Time: Dec 24 04:57:18 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Dec 24 04:54:59 2021
Response via : Initial Calibration

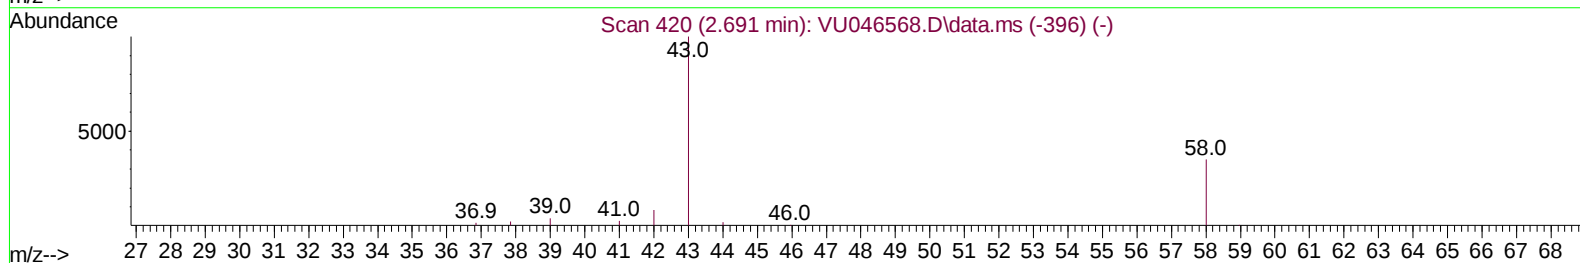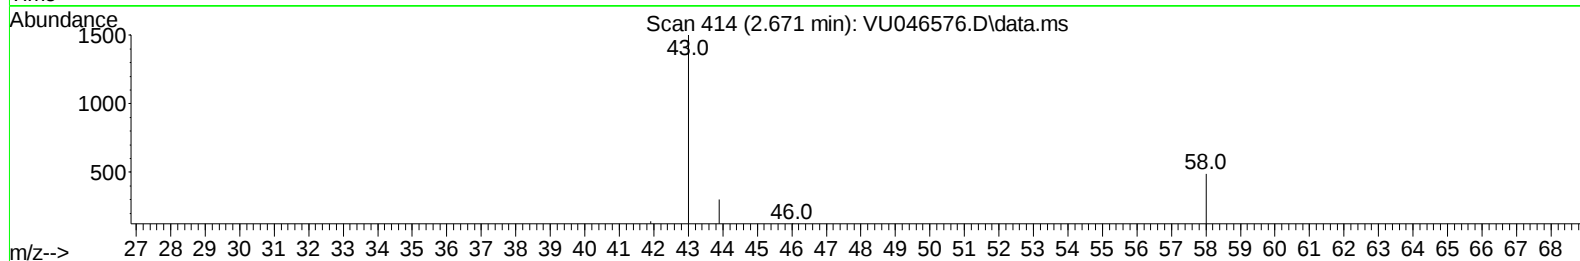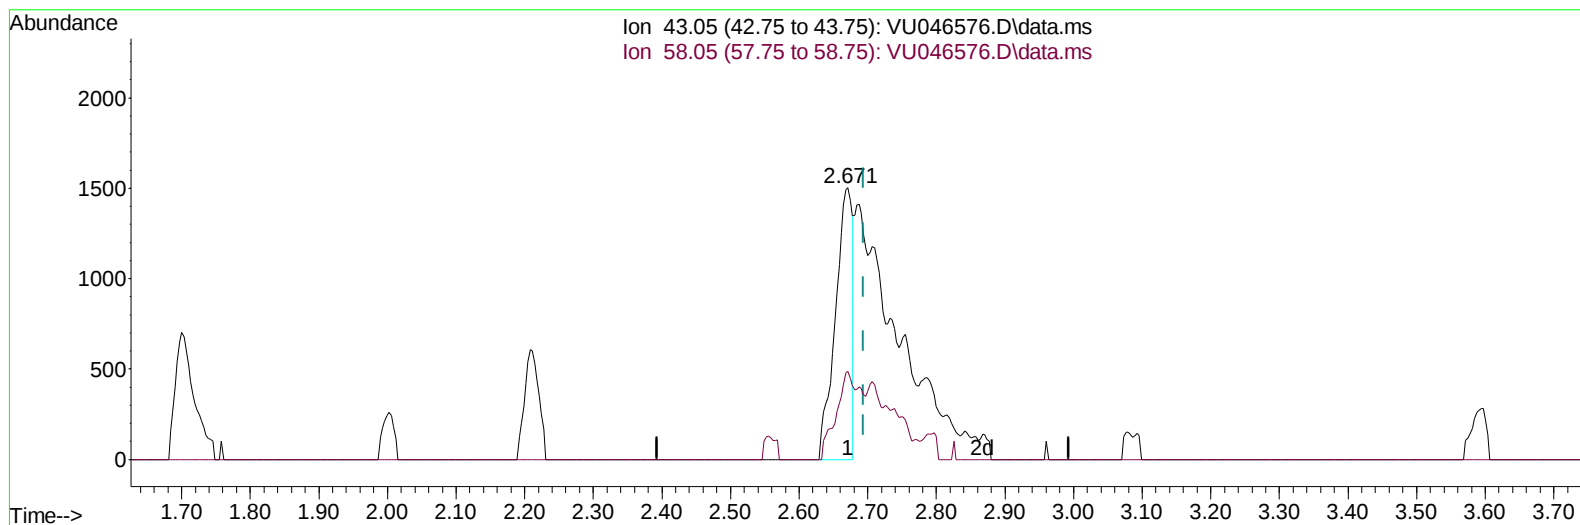

TIC: VU046576.D\data.ms

(13) Acetone (T)

2.671min (-0.023) 1.51 ug/L

response 2567

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	36.77
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122321\
Data File : VU046576.D
Acq On : 23 Dec 2021 19:25
Operator : SY/MD
Sample : M5175-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBBY5

Manual IntegrationsAPPROVED

Quant Time: Dec 24 04:57:18 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Dec 24 04:54:59 2021
Response via : Initial Calibration

Reviewed By :Amit Patel 12/24/2021
Supervised By :Semsettin Yesilyurt 01/02/2022

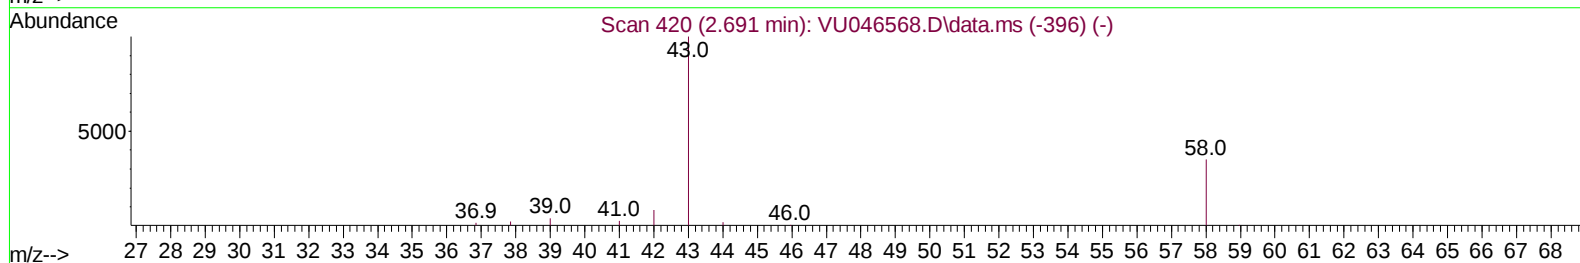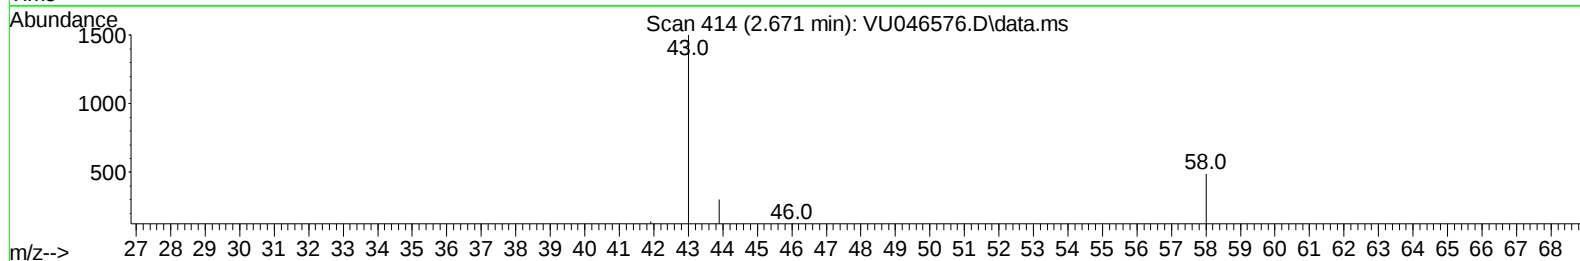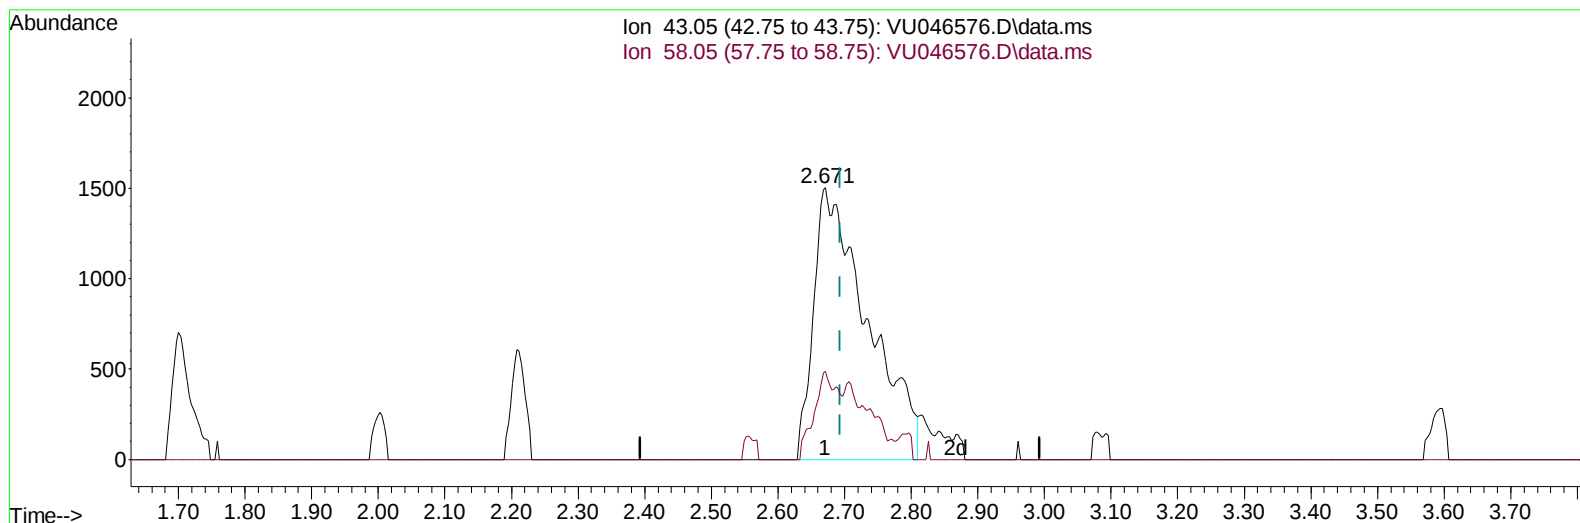

TIC: VU046576.D\data.ms

(13) Acetone (T)

2.671min (-0.023) 4.97 ug/L m

response 8441

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	11.18
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122321\
 Data File : VU046576.D
 Acq On : 23 Dec 2021 19:25
 Operator : SY/MD
 Sample : M5175-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBBY5

Manual IntegrationsAPPROVED

Quant Time: Dec 24 04:57:18 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Dec 24 04:54:59 2021
 Response via : Initial Calibration

Reviewed By :Amit Patel 12/24/2021
 Supervised By :Semsettin Yesilyurt 01/02/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	79233	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	78285	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	35826	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	20524	3.289	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	65.800%		
7) Chloroethane-d5	1.919	69	18765	3.818	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	76.400%		
11) 1,1-Dichloroethene-d2	2.571	65	9307	3.537	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	70.800%		
20) 2-Butanone-d5	4.655	46	98313	54.308	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	108.620%		
24) Chloroform-d	5.067	84	48140	4.210	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	84.200%		
26) 1,2-Dichloroethane-d4	5.706	65	29634	4.533	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	90.600%		
32) Benzene-d6	5.732	84	87530	4.011	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	80.200%		
36) 1,2-Dichloropropane-d6	6.694	67	28754	4.385	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	87.600%		
41) Toluene-d8	7.899	98	69568	3.512	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	70.200%		
43) trans-1,3-Dichloroprop...	8.179	79	11995	3.955	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	79.200%		
46) 2-Hexanone-d5	8.639	63	89120	50.049	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	100.100%		
56) 1,1,2,2-Tetrachloroeth...	10.758	84	31759	4.719	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	94.400%		
66) 1,2-Dichlorobenzene-d4	12.195	152	31382	4.755	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	95.200%		
Target Compounds						
					Qvalue	
13) Acetone	2.671	43	8441m	4.973	ug/L	
14) Carbon disulfide	2.800	76	4527	0.199	ug/L	100
22) cis-1,2-Dichloroethene	4.674	96	2056	0.253	ug/L	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122321\
Data File : VU046576.D
Acq On : 23 Dec 2021 19:25
Operator : SY/MD
Sample : M5175-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBBY5

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 12/24/2021
Supervised By :Semsettin Yesilyurt 01/02/2022

Quant Time: Dec 24 04:57:18 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Dec 24 04:54:59 2021
Response via : Initial Calibration

