


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122321\
Data File : VU046567.D
Acq On : 23 Dec 2021 13:35
Operator : SY/MD
Sample : BFB035
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB035

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122121WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Dec 30 04:21:35 2021

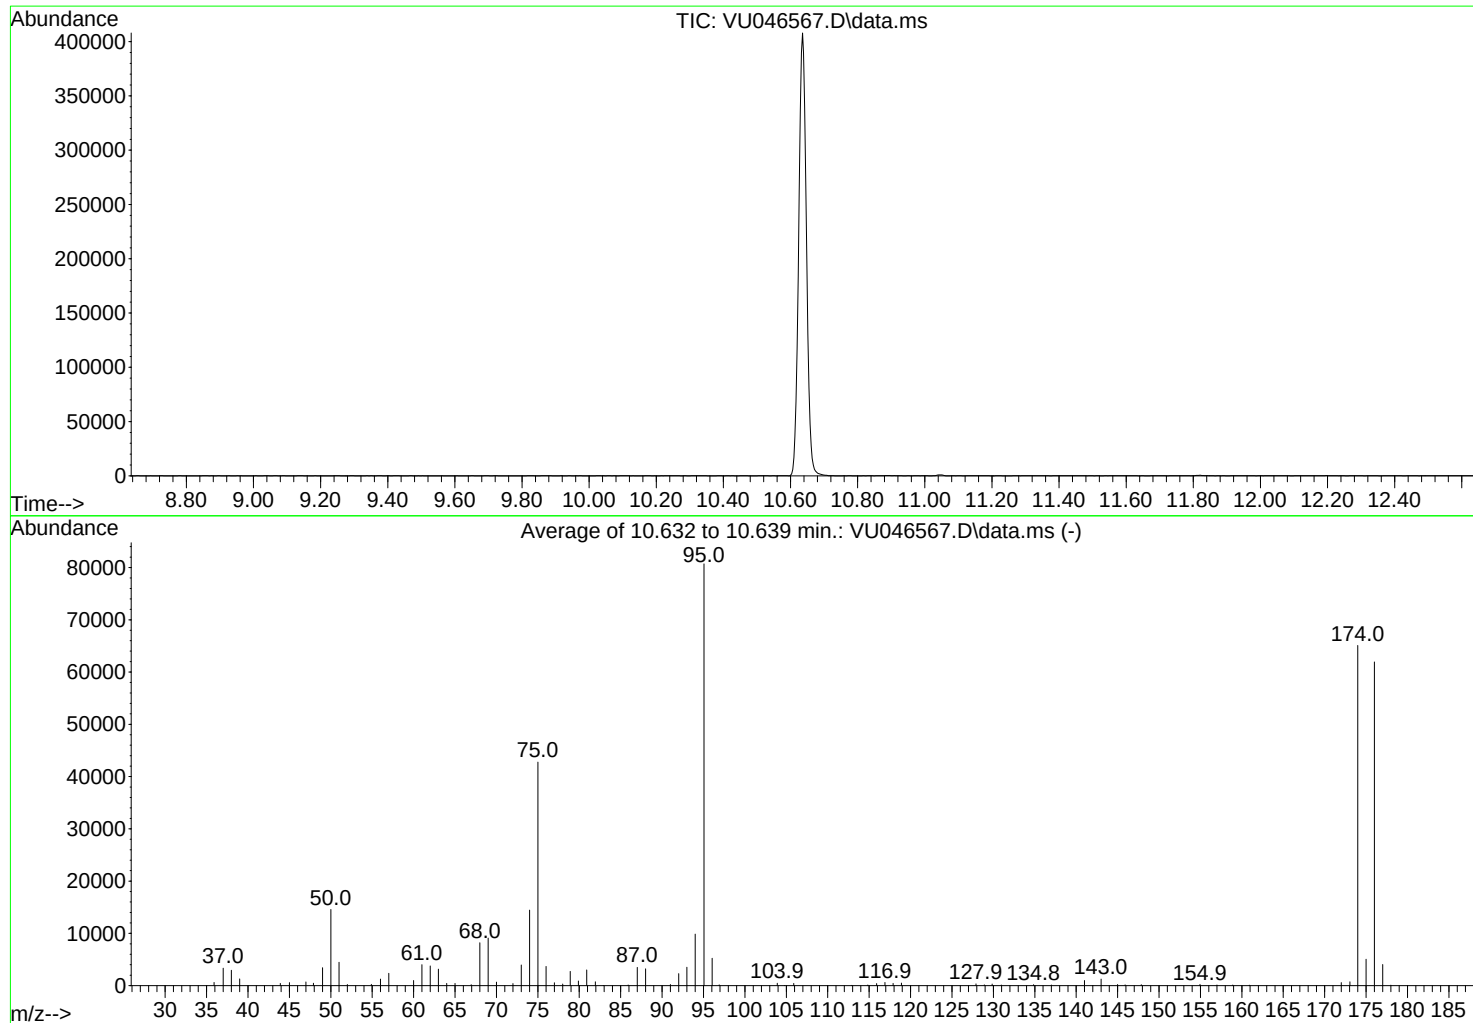

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	14566	PASS
75	95	30	80	53.0	42779	PASS
95	95	100	100	100.0	80707	PASS
96	95	5	9	6.5	5249	PASS
173	174	0.00	2	1.1	745	PASS
174	95	50	120	80.6	65080	PASS
175	174	5	9	7.8	5052	PASS
176	174	95	101	95.1	61920	PASS
177	176	5	9	6.5	4055	PASS

m/z	Abundance
44.00	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB035

m/z	Abundance
35.90	646.0
37.00	3398.0
38.00	2984.0
39.00	1345.0
43.90	473.0
45.00	592.0
47.00	726.0
47.90	441.0
49.00	3459.0
50.00	14484.0
51.00	4522.0
52.00	220.0
54.90	231.0
56.00	1302.0
57.00	2501.0
60.00	1041.0
61.00	4148.0
62.00	3836.0
63.00	3127.0
64.00	447.0
65.00	491.0
67.00	177.0
68.00	8256.0
69.00	9053.0
70.00	684.0
72.00	421.0
73.00	3982.0
74.00	14341.0
75.00	42720.0
76.00	3742.0
77.00	568.0
78.00	317.0
78.90	2729.0
79.90	908.0
80.90	2956.0
81.90	769.0
85.90	149.0
87.00	3291.0
88.00	2963.0
91.00	213.0
92.00	2298.0
93.00	3459.0
94.00	9665.0
95.10	79288.0
96.10	5211.0
96.90	166.0
103.90	491.0
104.80	100.0
105.90	470.0
112.90	112.0
114.80	132.0
115.90	368.0
116.90	617.0
117.90	443.0
118.90	479.0
127.90	322.0
129.00	159.0
129.90	355.0
131.00	110.0
134.90	184.0
137.00	122.0
141.00	880.0
142.00	105.0
143.00	1208.0
145.10	248.0
145.90	136.0
147.80	192.0
154.90	228.0
157.00	143.0
158.90	117.0
160.90	100.0
172.00	628.0
173.10	723.0
174.00	62840.0
175.00	5029.0
176.00	59744.0
177.00	4080.0

Instrument :
MSVOA_U
ClientSampleId :
BFB035

m/z	Abundance
35.90	640.0
37.00	3467.0
38.00	3054.0
39.00	1329.0
43.90	559.0
45.00	615.0
47.00	737.0
47.90	491.0
49.00	3572.0
50.00	14961.0
51.00	4612.0
52.00	223.0
54.90	240.0
56.00	1312.0
57.00	2446.0
60.00	1034.0
61.00	4140.0
62.00	3834.0
63.00	3236.0
64.00	451.0
65.00	440.0
66.90	207.0
68.00	8435.0
69.00	9478.0
70.00	691.0
72.00	387.0
73.00	4073.0
74.00	14797.0
75.00	44008.0
76.00	3757.0
77.00	566.0
78.00	330.0
78.90	2786.0
79.90	947.0
80.90	3100.0
82.00	768.0
85.90	140.0
87.00	3656.0
88.00	3280.0
91.00	226.0
92.00	2347.0
93.00	3625.0
94.00	10104.0
95.10	83264.0
96.10	5424.0
96.90	174.0
103.90	507.0
105.90	461.0
112.90	117.0
114.90	121.0
115.90	404.0
116.90	636.0
117.90	458.0
118.90	523.0
127.90	338.0
128.90	157.0
129.80	320.0
131.00	132.0
134.90	201.0
137.00	129.0
141.00	991.0
143.00	1293.0
145.00	217.0
145.90	150.0
147.90	206.0
155.00	261.0
157.00	123.0
158.90	145.0
160.90	116.0
172.00	599.0
173.00	775.0
174.00	67224.0
175.00	5236.0
176.00	63808.0
177.00	4162.0
178.00	122.0

Instrument :
MSVOA_U
ClientSampleId :
BFB035

m/z	Abundance
35.90	595.0
37.00	3198.0
38.00	2788.0
39.00	1171.0
43.90	561.0
45.00	552.0
47.00	707.0
47.90	476.0
49.00	3292.0
50.00	14253.0
51.00	4260.0
52.00	199.0
54.90	232.0
56.00	1167.0
57.00	2179.0
60.00	905.0
61.00	3774.0
62.00	3621.0
63.00	3148.0
64.00	373.0
65.00	397.0
67.00	209.0
68.00	7919.0
69.00	8785.0
70.00	612.0
72.00	364.0
73.00	3774.0
74.00	14199.0
75.00	41608.0
76.00	3488.0
77.00	508.0
78.00	294.0
78.90	2688.0
79.90	847.0
80.90	2989.0
82.00	708.0
82.90	107.0
85.90	109.0
87.00	3547.0
88.00	3406.0
91.00	211.0
92.00	2220.0
93.00	3516.0
94.00	9811.0
95.00	79568.0
96.00	5113.0
96.90	154.0
103.90	426.0
105.90	411.0
114.90	121.0
115.90	407.0
116.90	593.0
117.90	401.0
118.90	510.0
127.90	337.0
128.80	158.0
129.80	289.0
130.90	149.0
134.80	182.0
137.00	143.0
141.00	1039.0
143.00	1232.0
144.90	205.0
145.90	146.0
147.90	181.0
155.00	232.0
157.00	109.0
158.90	135.0
160.90	116.0
172.00	501.0
173.00	736.0
174.00	65176.0
175.00	4890.0
176.00	62208.0
177.00	3924.0
178.00	126.0

Instrument :
MSVOA_U
ClientSampleId :
BFB035