

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122322\
 Data File : VU052543.D
 Acq On : 23 Dec 2022 17:31
 Operator : JC/MD
 Sample : N6171-21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBQD7

Quant Time: Dec 24 03:57:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Dec 24 03:53:16 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	178127	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	176809	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	77122	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	61708	3.419	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.400%
7) Chloroethane-d5	1.916	69	65261	4.193	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	83.800%
11) 1,1-Dichloroethene-d2	2.568	65	28385	3.655	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.200%
20) 2-Butanone-d5	4.639	46	317435	56.724	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.440%
24) Chloroform-d	5.060	84	142041	4.665	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.400%
26) 1,2-Dichloroethane-d4	5.700	65	86929	4.922	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.400%
32) Benzene-d6	5.723	84	284953	4.701	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.000%
36) 1,2-Dichloropropane-d6	6.687	67	101708	4.874	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.400%
41) Toluene-d8	7.896	98	223649	4.395	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.800%
43) trans-1,3-Dichloroprop...	8.176	79	35495	4.968	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	99.400%
46) 2-Hexanone-d5	8.632	63	219725	56.206	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	112.420%
56) 1,1,2,2-Tetrachloroeth...	10.751	84	87505	4.939	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.800%
66) 1,2-Dichlorobenzene-d4	12.189	152	85344	5.435	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	108.800%
Target Compounds						
					Qvalue	
22) cis-1,2-Dichloroethene	4.658	96	3366	0.223	ug/L	96
34) Trichloroethene	6.543	95	8108	0.545	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122322\
Data File : VU052543.D
Acq On : 23 Dec 2022 17:31
Operator : JC/MD
Sample : N6171-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBQD7

Quant Time: Dec 24 03:57:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Dec 24 03:53:16 2022
Response via : Initial Calibration




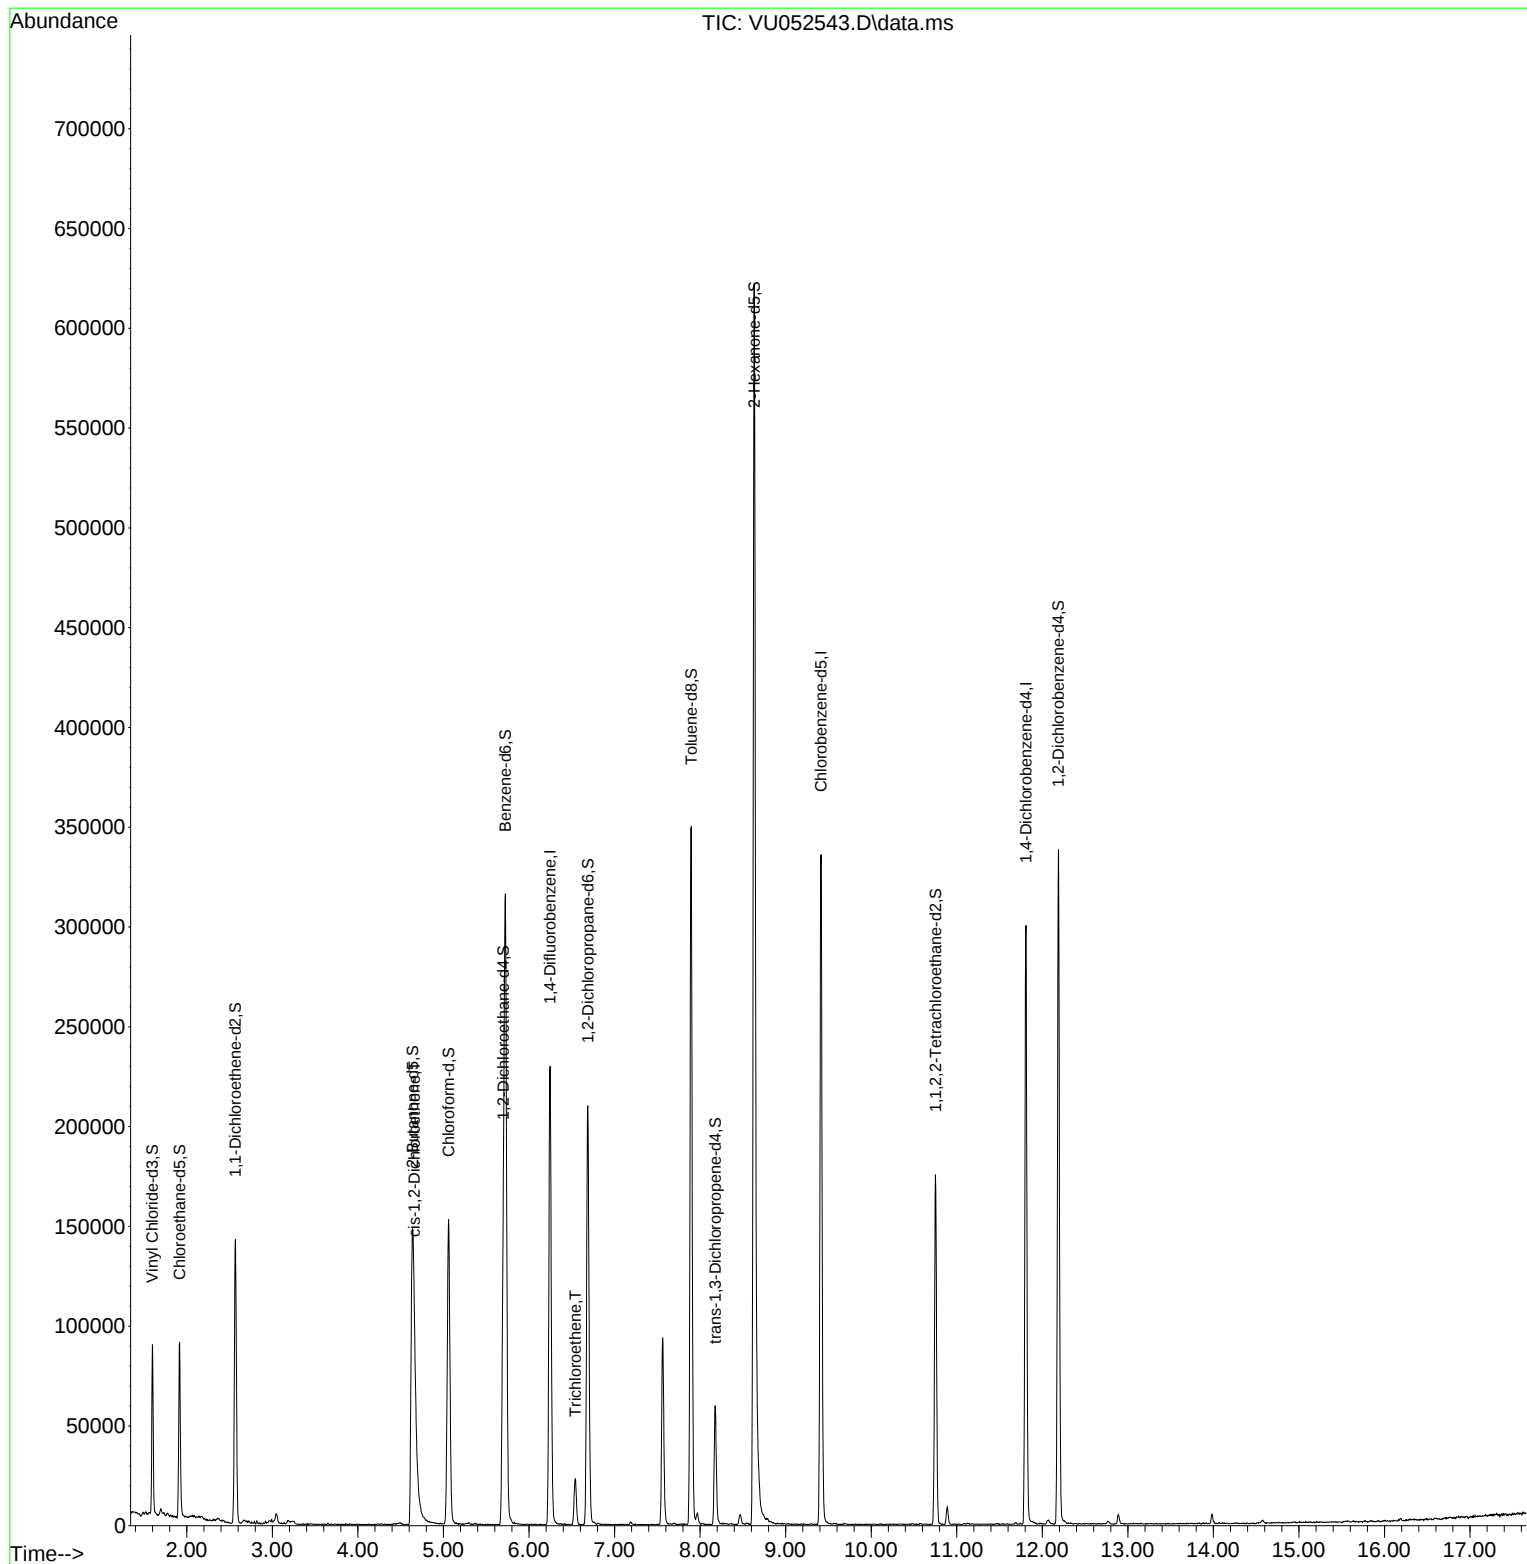


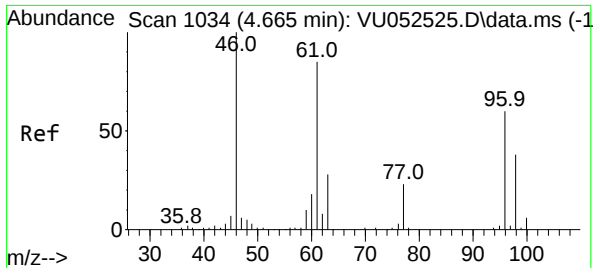

#22
cis-1,2-Dichloroethene
Concen: 0.223 ug/L
RT: 4.658 min Scan# 1032
Delta R.T. -0.006 min
Lab File: VU052543.D
Acq: 23 Dec 2022 17:31

Instrument :
MSVOA_U
ClientSampleId :
GBQD7

Tgt Ion: 96 Resp: 3366
Ion Ratio Lower Upper
96 100
61 132.6 96.9 180.1
98 66.7 44.7 83.1

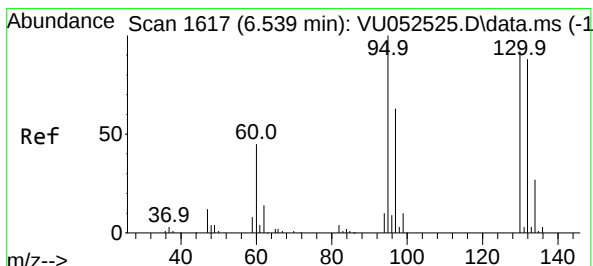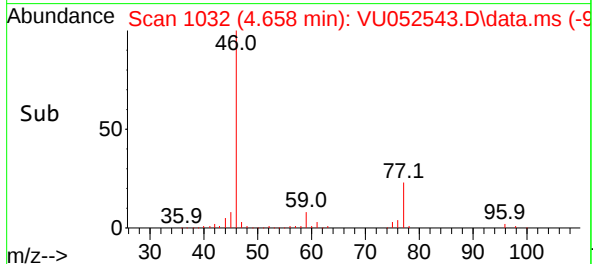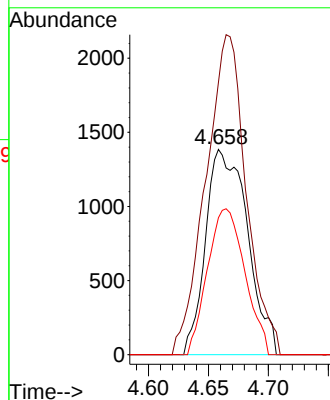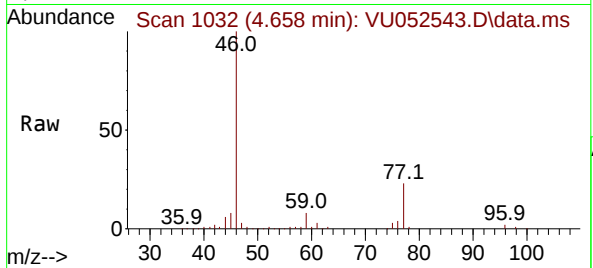

#34
Trichloroethene
Concen: 0.545 ug/L
RT: 6.543 min Scan# 1618
Delta R.T. 0.003 min
Lab File: VU052543.D
Acq: 23 Dec 2022 17:31

Tgt Ion: 95 Resp: 8108
Ion Ratio Lower Upper
95 100
97 69.1 46.3 86.1
132 85.8 63.9 118.7
130 92.6 65.9 122.5

