

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122322\
 Data File : VU052529.D
 Acq On : 23 Dec 2022 12:06
 Operator : JC/MD
 Sample : N6188-08DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0L45DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052529.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	72	81	97	rVB2	145991	175791	14.06%	1.940%
2	1.916	169	179	198	rVB	106469	144303	11.54%	1.593%
3	2.568	370	382	398	rBV	189570	309887	24.79%	3.420%
4	3.044	518	530	547	rBV3	27992	56424	4.51%	0.623%
5	4.661	1010	1033	1067	rBV2	356956	1095307	87.61%	12.089%
6	5.060	1140	1157	1185	rBV	172010	382690	30.61%	4.224%
7	5.722	1342	1363	1390	rBV2	366613	959761	76.77%	10.593%
8	6.247	1510	1526	1550	rBV	267094	508481	40.67%	5.612%
9	6.539	1604	1617	1640	rBV	262248	496584	39.72%	5.481%
10	6.687	1649	1663	1683	rBV	239055	464635	37.16%	5.128%
11	7.562	1923	1935	1954	rBV	107712	191607	15.33%	2.115%
12	7.896	2023	2039	2052	rBV	414916	721015	57.67%	7.958%
13	7.967	2052	2061	2076	rVB	57820	102301	8.18%	1.129%
14	8.176	2115	2126	2142	rBV2	66422	115043	9.20%	1.270%
15	8.632	2254	2268	2308	rBV2	612584	1250224	100.00%	13.799%
16	9.414	2497	2511	2536	rBV	366293	609536	48.75%	6.727%
17	10.751	2915	2927	2947	rBV	184594	298068	23.84%	3.290%
18	10.889	2962	2970	2981	rVB2	8156	13389	1.07%	0.148%
19	11.809	3241	3256	3278	rBV	337627	542382	43.38%	5.986%
20	12.188	3362	3374	3394	rBV	382173	622939	49.83%	6.875%




Sum of corrected areas: 9060367

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122322\
Data File : VU052529.D
Acq On : 23 Dec 2022 12:06
Operator : JC/MD
Sample : N6188-08DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L45DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

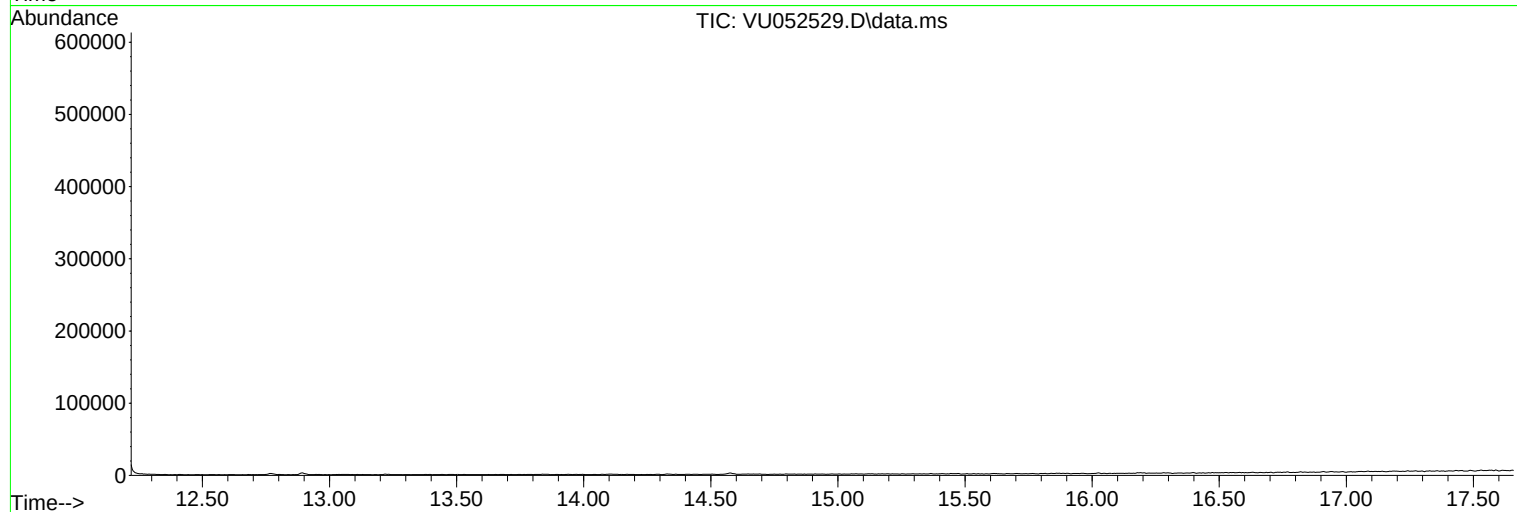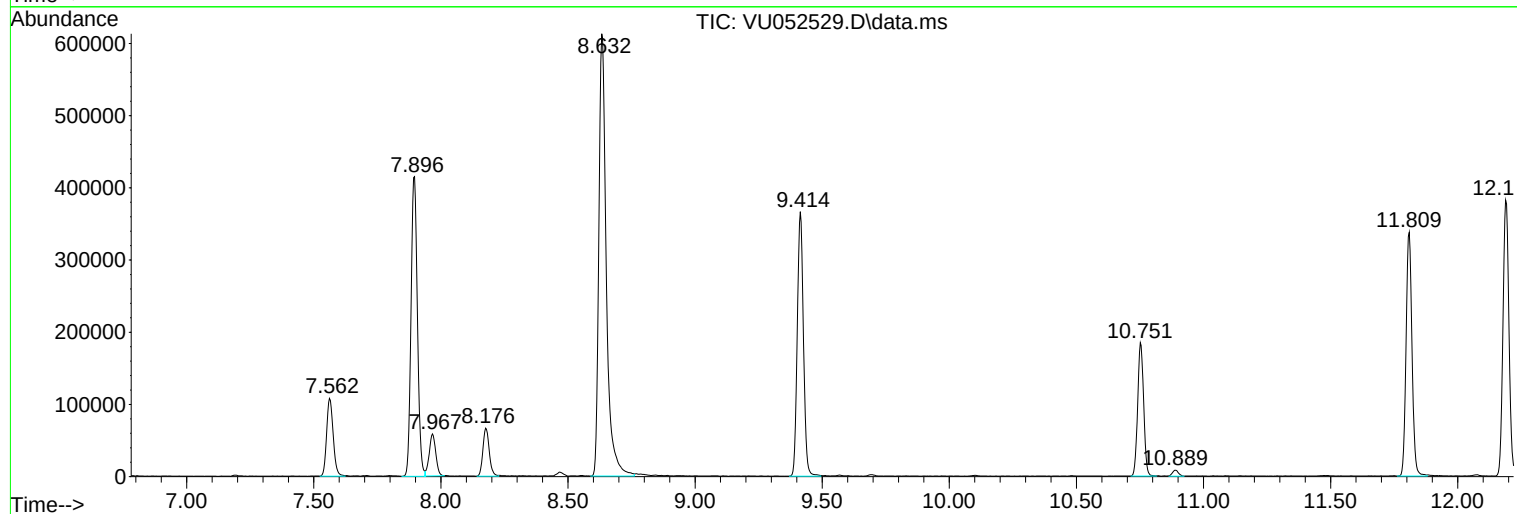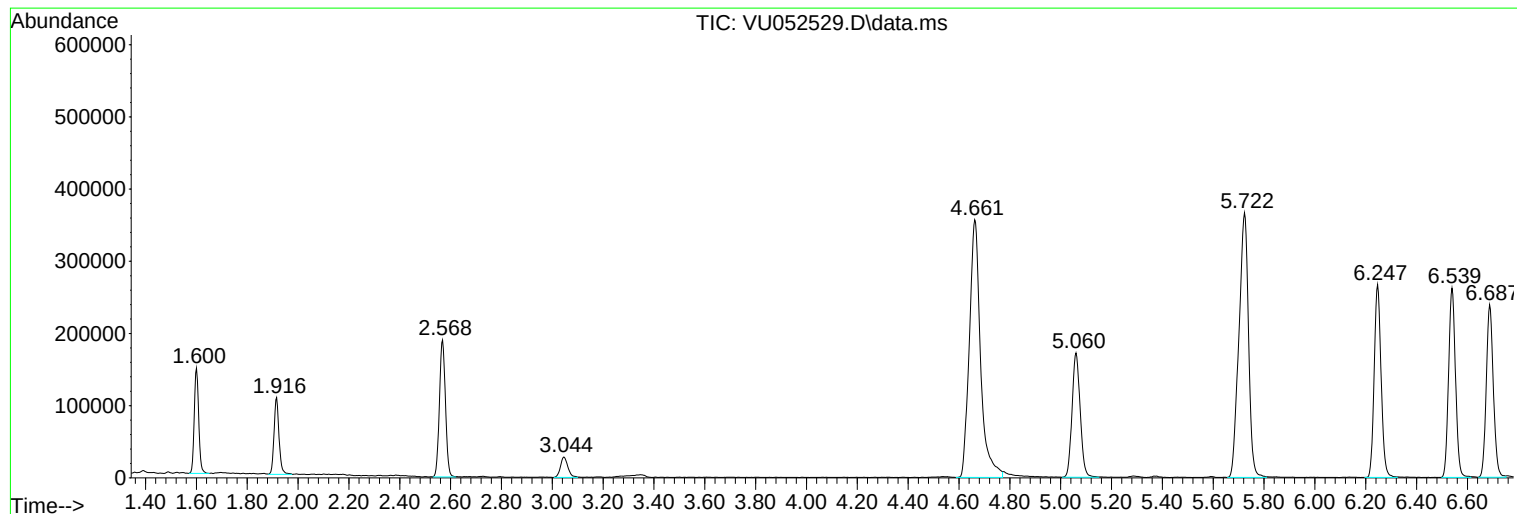

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122322\
Data File : VU052529.D
Acq On : 23 Dec 2022 12:06
Operator : JC/MD
Sample : N6188-08DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L45DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122322\
Data File : VU052529.D
Acq On : 23 Dec 2022 12:06
Operator : JC/MD
Sample : N6188-08DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L45DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
