

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122322\
 Data File : VU052530.D
 Acq On : 23 Dec 2022 12:29
 Operator : JC/MD
 Sample : N6188-05DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0L39DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052530.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	95	rVB	99676	114306	9.48%	1.390%
2	1.916	170	179	195	rVB	96426	128316	10.65%	1.561%
3	2.568	369	382	400	rVB	166543	278710	23.12%	3.390%
4	3.044	520	530	547	rVB2	13595	26624	2.21%	0.324%
5	4.652	1012	1030	1089	rBV3	143659	589362	48.90%	7.168%
6	5.060	1141	1157	1179	rBV	158778	352326	29.23%	4.285%
7	5.723	1338	1363	1393	rBV3	333208	881682	73.15%	10.724%
8	6.247	1512	1526	1549	rBV	252528	486307	40.35%	5.915%
9	6.539	1603	1617	1640	rBV	421221	792237	65.73%	9.636%
10	6.687	1650	1663	1682	rBV	221505	430848	35.74%	5.240%
11	7.562	1923	1935	1959	rBV	99713	178850	14.84%	2.175%
12	7.896	2025	2039	2055	rBV	376530	655321	54.37%	7.971%
13	7.967	2055	2061	2072	rVB2	9566	15675	1.30%	0.191%
14	8.176	2113	2126	2144	rBV	62934	108463	9.00%	1.319%
15	8.632	2256	2268	2305	rBV2	602273	1205342	100.00%	14.661%
16	9.414	2498	2511	2532	rBV	360245	596737	49.51%	7.258%
17	10.751	2915	2927	2942	rBV	173147	283518	23.52%	3.448%
18	11.809	3244	3256	3271	rBV	328216	521295	43.25%	6.341%
19	12.189	3361	3374	3396	rBV	354548	575699	47.76%	7.002%




Sum of corrected areas: 8221618

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122322\
Data File : VU052530.D
Acq On : 23 Dec 2022 12:29
Operator : JC/MD
Sample : N6188-05DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L39DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

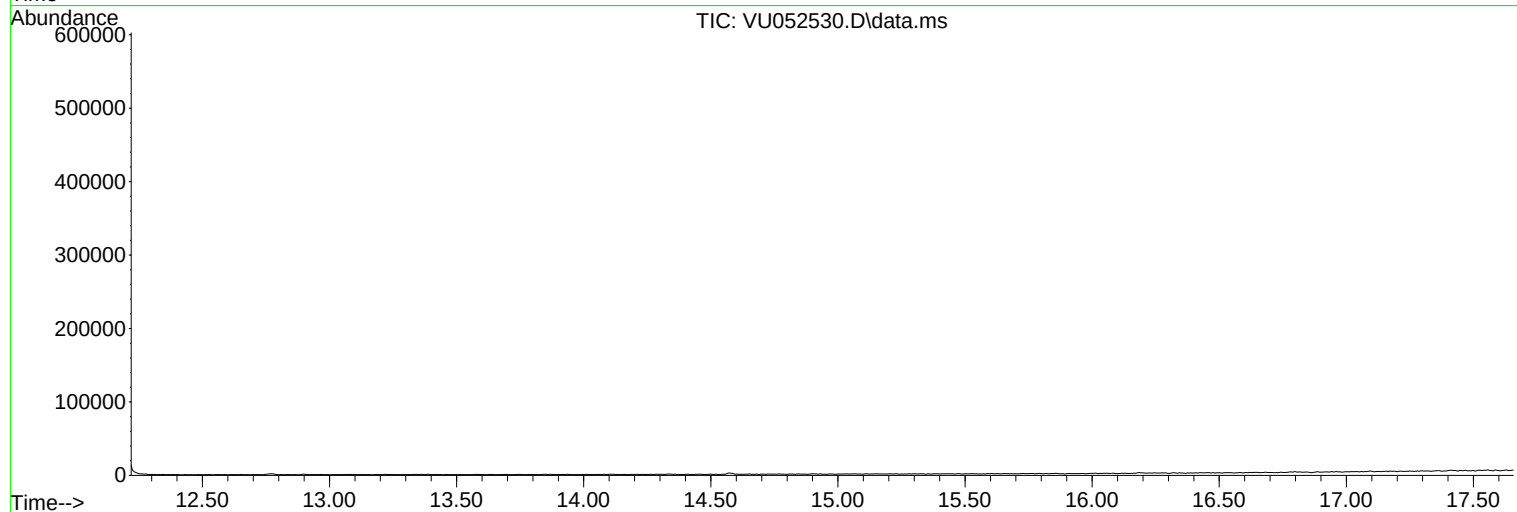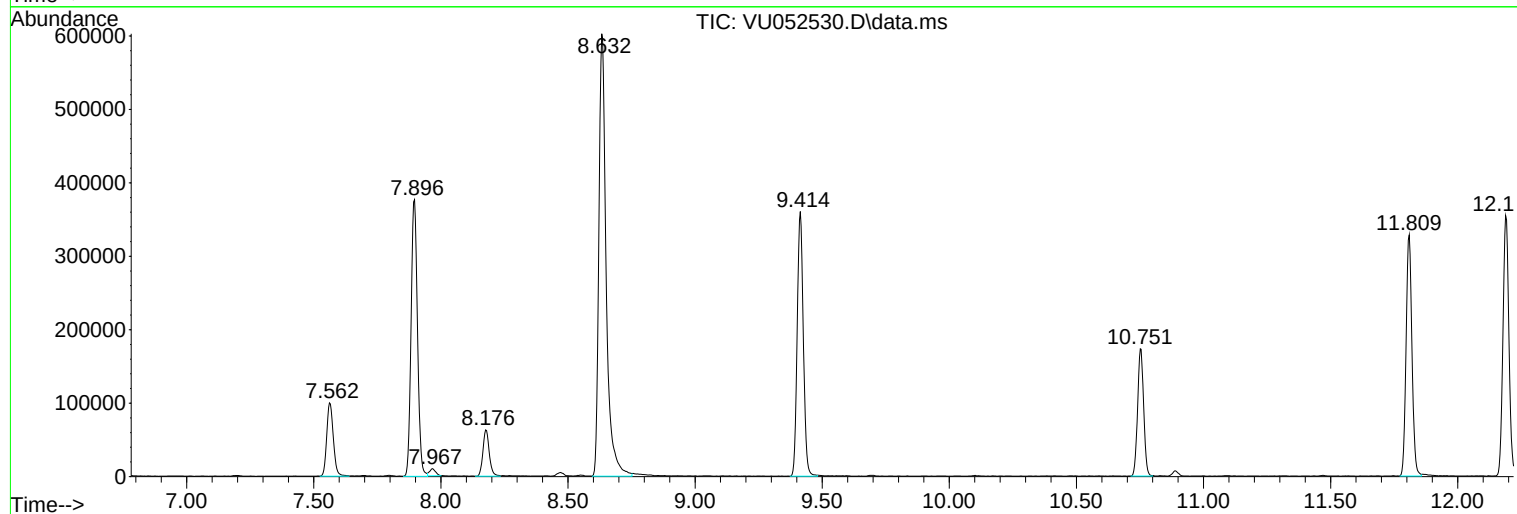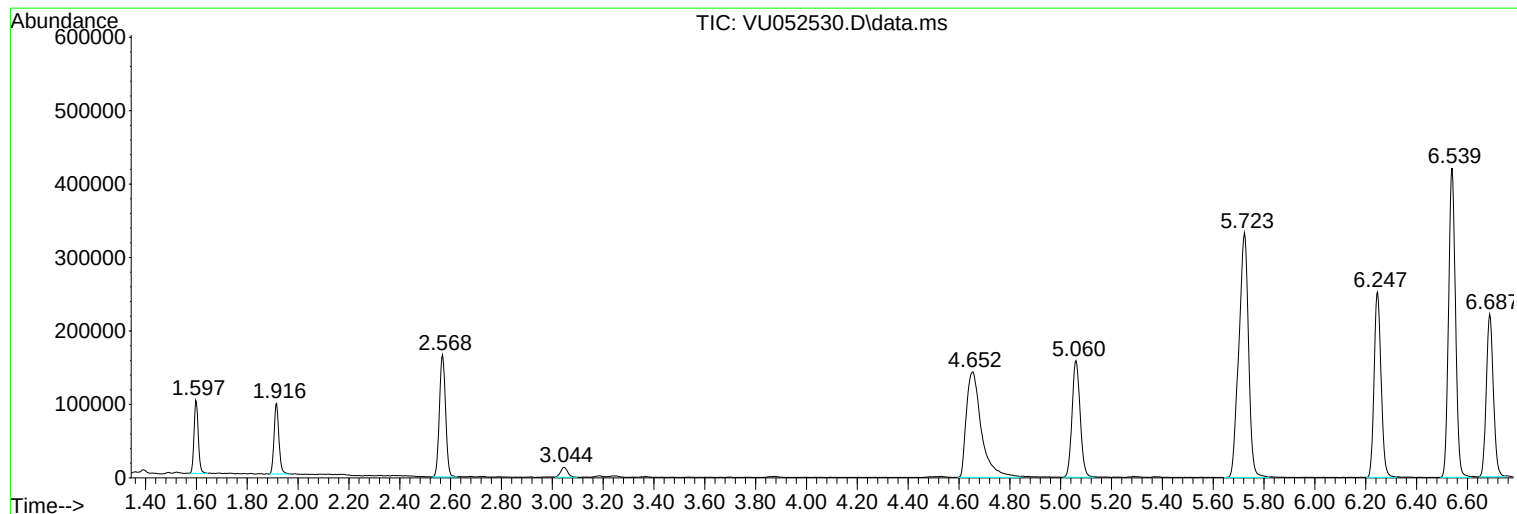

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122322\
Data File : VU052530.D
Acq On : 23 Dec 2022 12:29
Operator : JC/MD
Sample : N6188-05DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L39DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122322\
Data File : VU052530.D
Acq On : 23 Dec 2022 12:29
Operator : JC/MD
Sample : N6188-05DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L39DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc