

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122322\
 Data File : VU052533.D
 Acq On : 23 Dec 2022 13:40
 Operator : JC/MD
 Sample : VIBLK138
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK138

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052533.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	95	rVB	94728	107946	8.68%	1.476%
2	1.912	170	178	195	rBV	92836	124725	10.03%	1.705%
3	2.568	369	382	395	rBV	158597	258502	20.79%	3.535%
4	3.044	520	530	549	rVB2	9110	17844	1.44%	0.244%
5	4.658	1016	1032	1078	rBV2	94343	501375	40.33%	6.855%
6	5.060	1141	1157	1183	rVB	160020	352567	28.36%	4.821%
7	5.722	1342	1363	1394	rBV2	332846	884859	71.17%	12.099%
8	6.247	1511	1526	1550	rBV	241984	463724	37.30%	6.341%
9	6.539	1605	1617	1630	rBV4	14565	29767	2.39%	0.407%
10	6.687	1649	1663	1687	rBV	215547	430714	34.64%	5.889%
11	7.562	1924	1935	1954	rBV2	99338	178566	14.36%	2.442%
12	7.896	2025	2039	2056	rBV	370198	640365	51.50%	8.756%
13	8.176	2112	2126	2144	rBV	63407	110382	8.88%	1.509%
14	8.636	2254	2269	2301	rBV	585628	1243327	100.00%	17.000%
15	9.414	2498	2511	2533	rBV	345226	575526	46.29%	7.869%
16	10.751	2913	2927	2947	rBV	179374	291963	23.48%	3.992%
17	10.889	2959	2970	2980	rBV2	8501	13296	1.07%	0.182%
18	11.809	3244	3256	3281	rBV	322276	512363	41.21%	7.006%
19	12.188	3361	3374	3394	rBV	349817	575758	46.31%	7.872%




Sum of corrected areas: 7313569

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122322\
Data File : VU052533.D
Acq On : 23 Dec 2022 13:40
Operator : JC/MD
Sample : VIBLK138
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK138

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

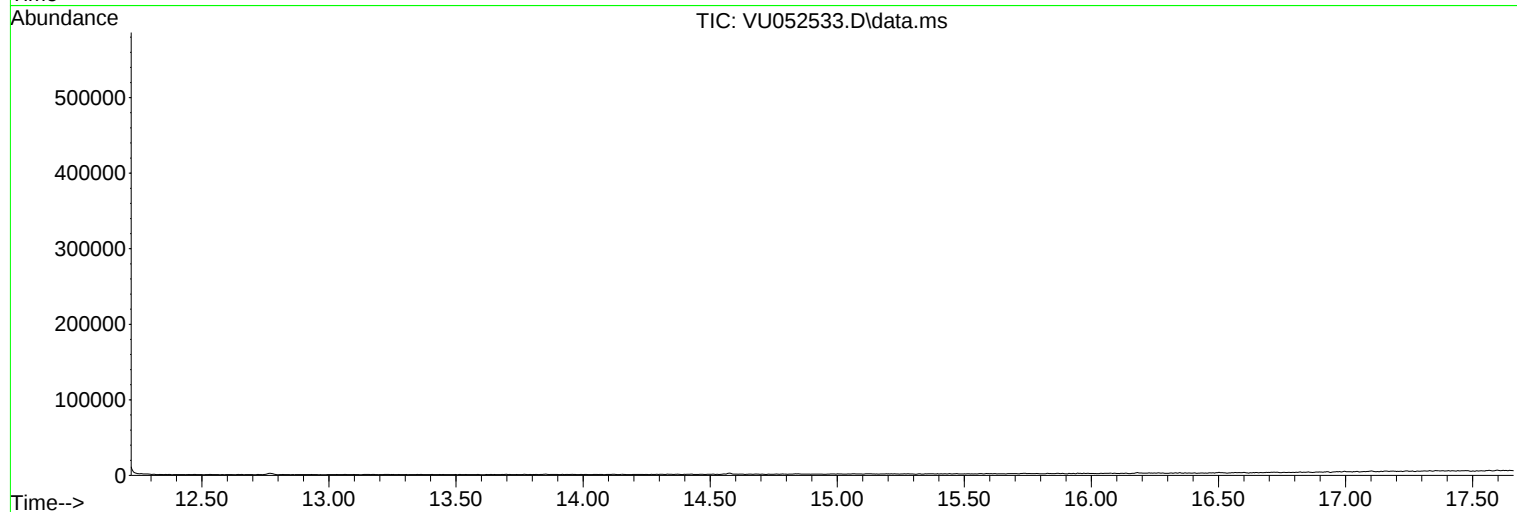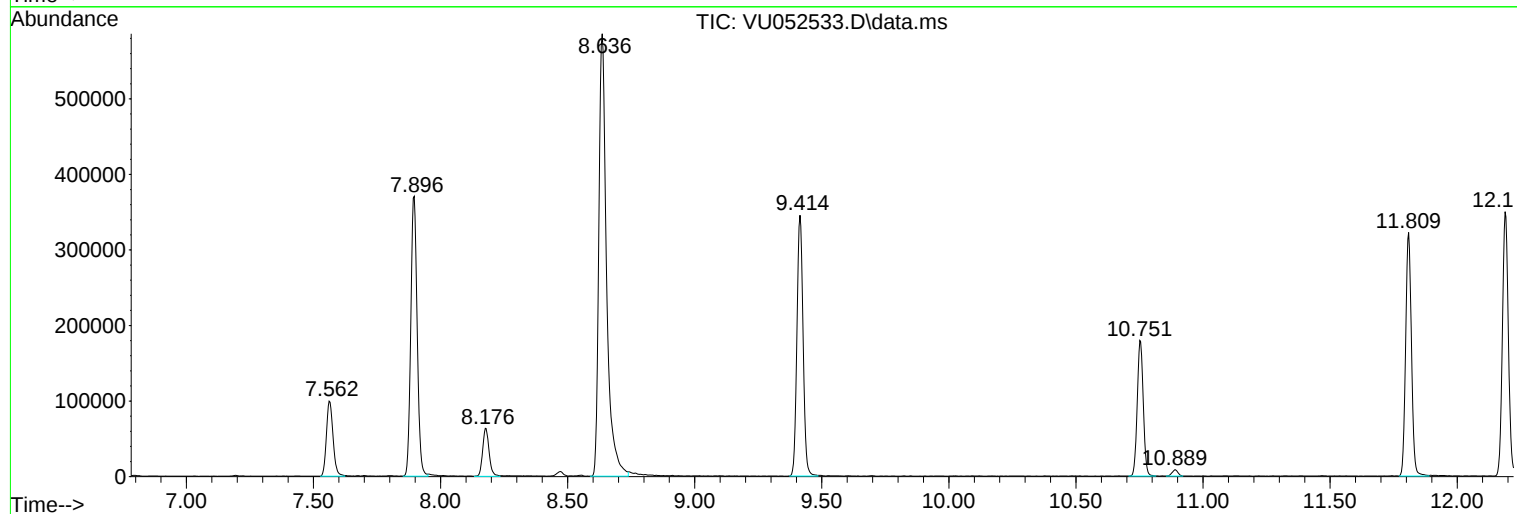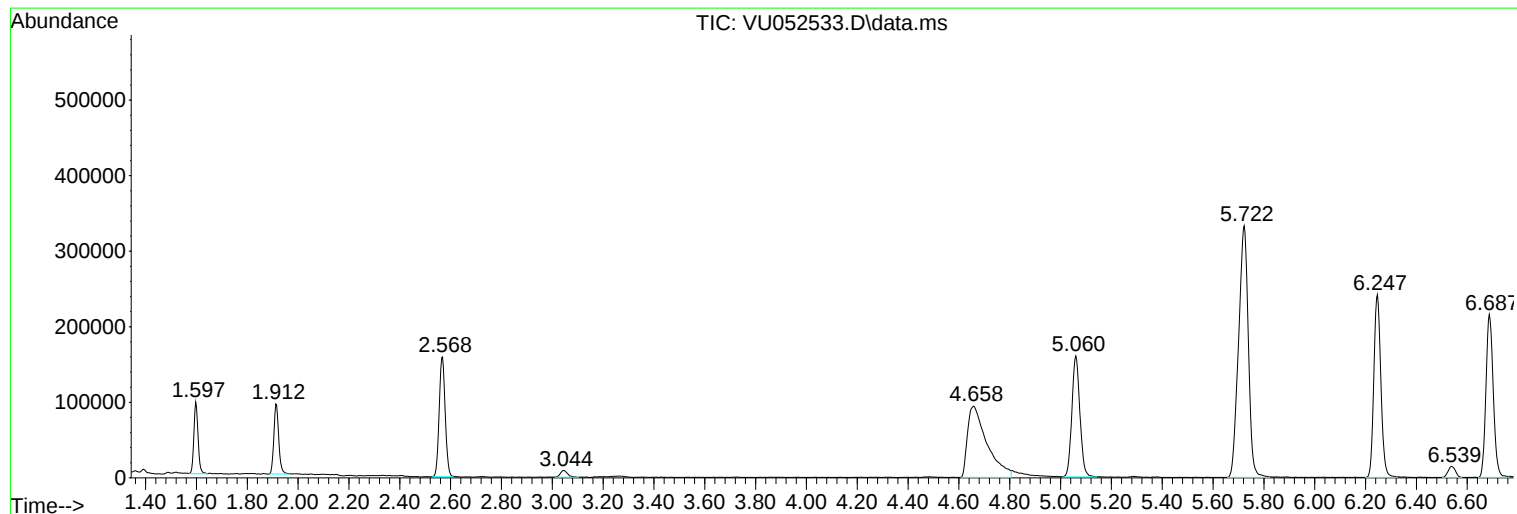

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122322\
Data File : VU052533.D
Acq On : 23 Dec 2022 13:40
Operator : JC/MD
Sample : VIBLK138
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK138

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122322\
Data File : VU052533.D
Acq On : 23 Dec 2022 13:40
Operator : JC/MD
Sample : VIBLK138
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK138

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
