


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122322\
 Data File : VU052524.D
 Acq On : 23 Dec 2022 08:55
 Operator : JC/MD
 Sample : BFB184
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB184

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122022WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Dec 28 01:18:16 2022

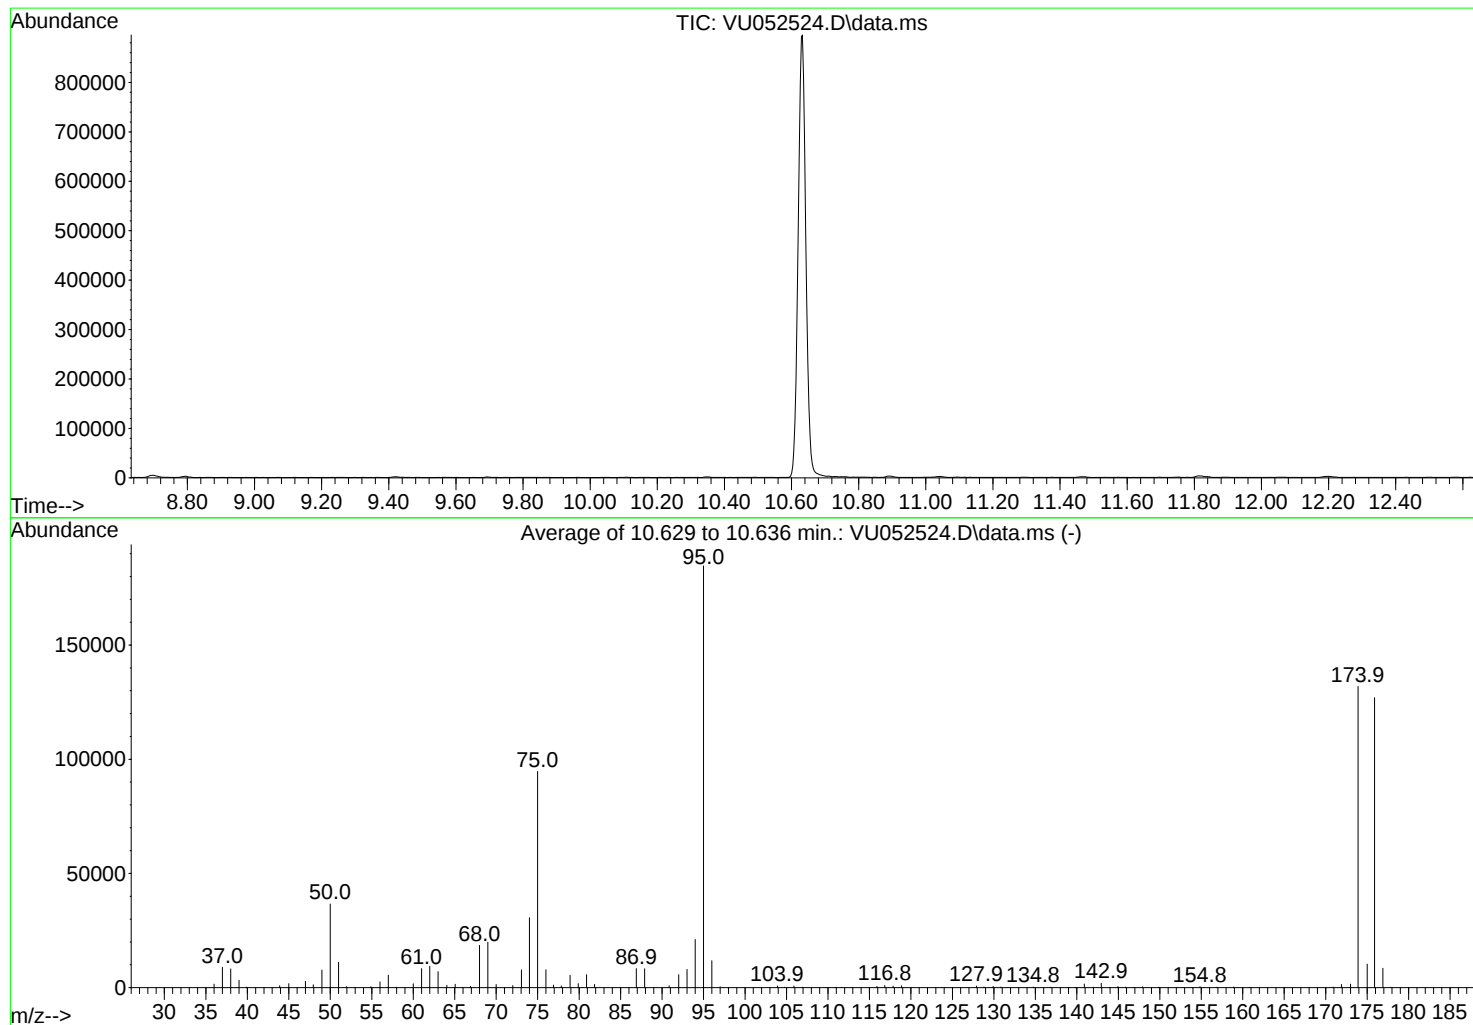

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	36616	PASS
75	95	30	80	51.3	94653	PASS
95	95	100	100	100.0	184683	PASS
96	95	5	9	6.4	11779	PASS
173	174	0.00	2	1.2	1554	PASS
174	95	50	120	71.4	131907	PASS
175	174	5	9	7.8	10285	PASS
176	174	95	101	96.2	126949	PASS
177	176	5	9	6.7	8511	PASS

m/z	Abundance
39.90	428.0
43.90	583.0

Instrument :
MSVOA_U
ClientSampleId :
BFB184

m/z	Abundance
36.00	1721.0
37.00	9399.0
38.00	8631.0
39.00	3512.0
40.00	612.0
44.00	1323.0
45.00	1749.0
46.00	283.0
47.00	3099.0
47.90	1374.0
49.00	8006.0
50.00	38760.0
51.00	11767.0
51.90	548.0
52.90	186.0
54.90	460.0
56.00	2661.0
57.00	5504.0
58.00	209.0
60.00	1708.0
61.00	8682.0
62.00	9674.0
63.00	7123.0
64.00	1204.0
65.10	1553.0
65.90	102.0
66.90	567.0
68.00	19376.0
69.00	20768.0
70.00	1350.0
72.00	899.0
73.00	8298.0
74.00	32280.0
75.00	98664.0
76.00	8228.0
76.90	1070.0
77.80	853.0
78.90	5464.0
79.90	1794.0
80.90	5974.0
81.80	1378.0
85.90	193.0
86.90	8617.0
87.90	8407.0
90.80	817.0
92.00	5850.0
93.00	8479.0
94.00	21848.0
95.00	189632.0
96.00	12208.0
97.00	282.0
103.90	751.0
104.80	219.0
105.90	837.0
107.00	188.0
109.70	108.0
110.80	132.0
111.70	124.0
112.90	144.0
114.70	146.0
115.90	530.0
116.90	1035.0
117.80	728.0
118.90	869.0
126.00	126.0
127.90	684.0
128.80	234.0
129.90	656.0
130.80	250.0
134.80	250.0
136.90	253.0
139.00	113.0
139.80	115.0
140.90	1641.0
142.00	286.0
143.00	1893.0
144.00	130.0
144.90	566.0
145.90	359.0
147.80	423.0
149.80	156.0
154.80	406.0
157.00	198.0
158.90	271.0
160.90	184.0
170.90	295.0
171.90	1466.0
173.00	1644.0
173.90	133184.0
175.00	10544.0
175.90	127960.0
176.90	8621.0

Instrument :
MSVOA_U
ClientSampleId :
BFB184

177.80

226.0

Instrument :
MSVOA_U
ClientSampleId :
BFB184

m/z	Abundance
36.00	1585.0
37.00	9125.0
38.00	8518.0
39.00	3346.0
40.00	633.0
43.90	1481.0
45.00	1854.0
46.00	246.0
47.00	2882.0
47.90	1295.0
49.00	7936.0
50.00	37768.0
51.00	11377.0
51.90	467.0
53.00	179.0
54.90	447.0
56.00	2550.0
57.00	5765.0
58.00	186.0
60.00	1758.0
61.00	8538.0
62.00	9713.0
63.00	7280.0
64.10	1050.0
65.10	1538.0
66.00	122.0
66.90	540.0
68.00	19112.0
69.00	20560.0
70.00	1485.0
72.00	994.0
73.00	8072.0
74.00	31656.0
75.00	97736.0
76.00	8096.0
76.90	1157.0
77.90	805.0
78.90	5587.0
79.90	1820.0
80.90	5894.0
81.90	1516.0
86.00	148.0
86.90	8681.0
87.90	8578.0
90.80	860.0
92.00	5922.0
93.00	8255.0
94.00	21776.0
95.00	190848.0
96.00	12236.0
97.00	344.0
103.90	837.0
104.70	201.0
105.90	791.0
106.90	203.0
109.70	118.0
110.80	122.0
111.60	146.0
112.90	174.0
114.70	118.0
115.90	524.0
116.90	1019.0
117.90	752.0
118.90	839.0
123.70	111.0
125.90	134.0
127.90	745.0
128.80	265.0
129.90	567.0
130.80	266.0
134.70	285.0
136.80	205.0
140.90	1671.0
142.00	228.0
143.00	1957.0
144.00	123.0
144.90	508.0
145.90	297.0
146.80	112.0
147.90	367.0
149.80	139.0
152.90	100.0
153.90	116.0
154.90	435.0
156.90	177.0
158.90	314.0
160.80	181.0
170.90	270.0
171.90	1427.0
173.00	1576.0
173.90	136256.0
175.00	10671.0

Instrument :
MSVOA_U
ClientSampleId :
BFB184

175.90	131136.0
176.90	8841.0
177.90	234.0

Instrument :
MSVOA_U
ClientSampleId :
BFB184

m/z	Abundance
36.00	1386.0
37.00	8151.0
38.00	7357.0
39.00	2911.0
39.90	605.0
43.90	1546.0
45.00	1607.0
47.00	2328.0
48.00	1089.0
49.00	7263.0
50.00	33320.0
51.00	10083.0
52.00	360.0
53.00	147.0
54.90	431.0
56.00	2329.0
57.00	5145.0
57.90	159.0
60.00	1603.0
61.00	7742.0
62.00	8646.0
63.00	6613.0
64.10	855.0
65.00	1326.0
66.00	143.0
66.90	496.0
68.00	16992.0
69.00	18408.0
70.00	1465.0
72.00	939.0
73.10	7074.0
74.00	27864.0
75.00	87560.0
76.00	7147.0
76.90	1185.0
77.90	746.0
78.90	5111.0
79.90	1665.0
80.90	5125.0
81.90	1407.0
86.00	117.0
86.90	7679.0
87.90	7748.0
90.90	759.0
92.00	5321.0
93.00	7233.0
94.00	19664.0
95.00	173568.0
96.00	10892.0
97.00	347.0
103.90	804.0
104.80	207.0
105.90	668.0
106.90	193.0
110.90	117.0
111.60	120.0
112.90	173.0
115.90	544.0
116.80	938.0
117.90	671.0
118.80	776.0
123.70	105.0
127.90	707.0
128.80	300.0
129.90	489.0
130.90	257.0
134.70	261.0
136.80	194.0
140.90	1579.0
142.10	159.0
142.90	1912.0
143.90	115.0
145.00	390.0
145.90	217.0
146.90	109.0
148.00	336.0
149.90	129.0
152.90	113.0
154.90	400.0
156.80	203.0
158.90	257.0
160.80	160.0
170.90	205.0
171.90	1333.0
173.00	1442.0
173.90	126280.0
175.00	9639.0
175.90	121752.0
176.90	8072.0
177.90	209.0

Instrument :
MSVOA_U
ClientSampleId :
BFB184