
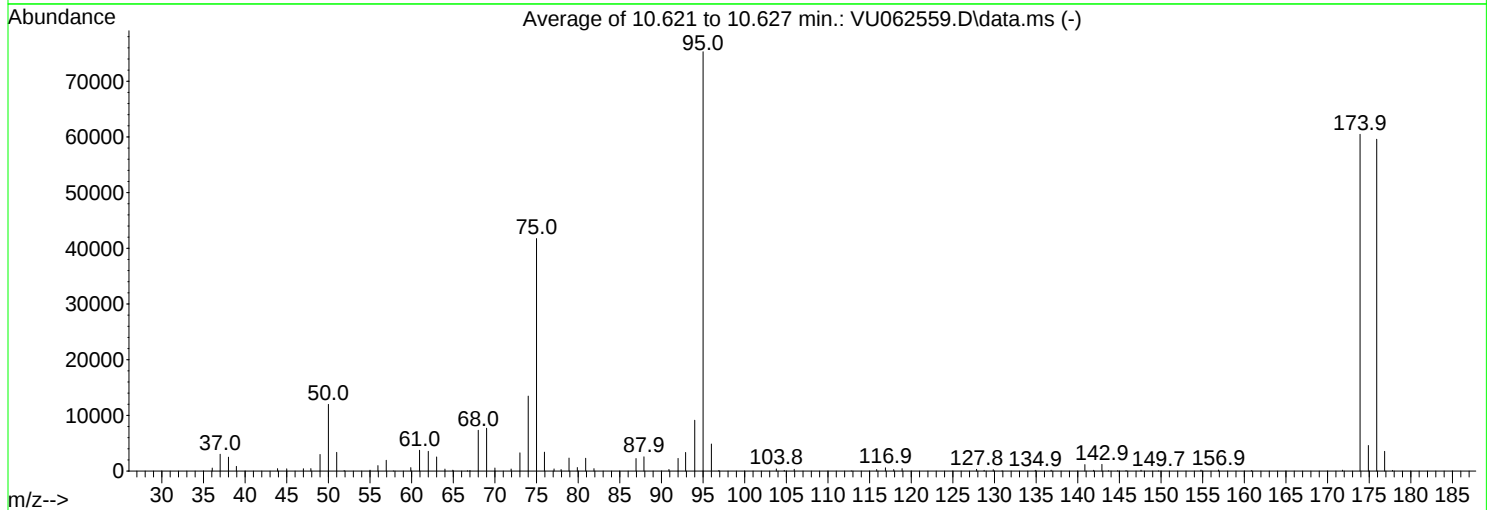


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122324\
Data File : VU062559.D
Acq On : 23 Dec 2024 08:55
Operator : MD/SY
Sample : BFB052
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB052

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Dec 27 21:56:24 2024

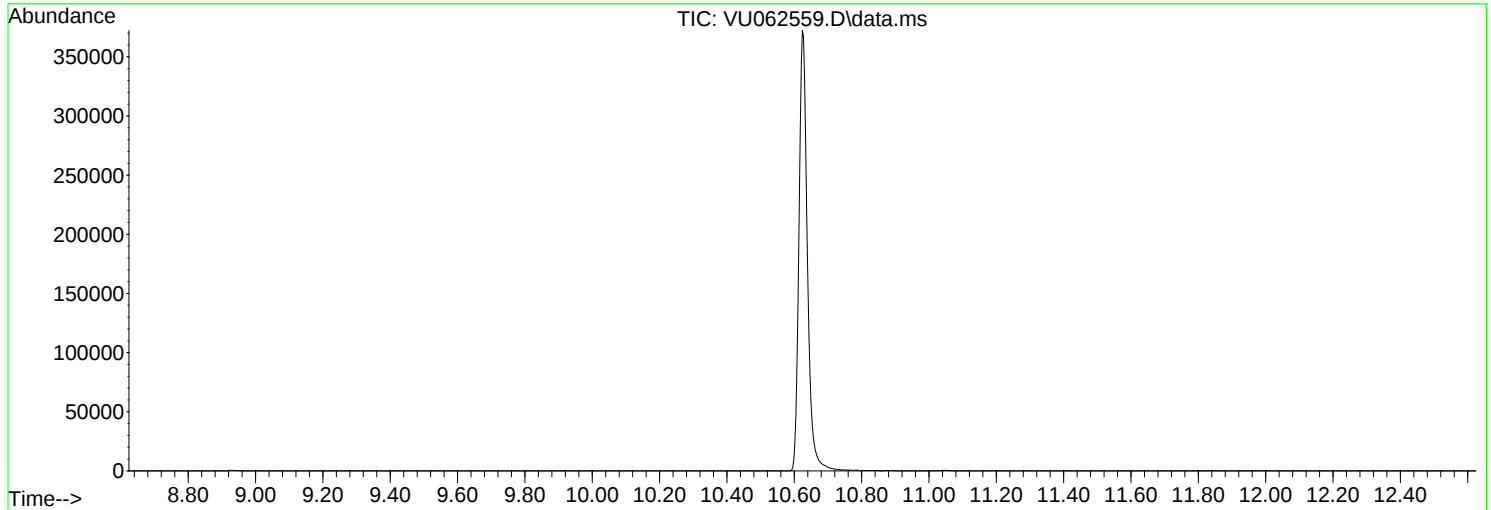

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	11980	PASS
75	95	30	80	55.4	41749	PASS
95	95	100	100	100.0	75299	PASS
96	95	5	9	6.5	4864	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.3	60475	PASS
175	174	5	9	7.6	4597	PASS
176	174	95	101	98.5	59589	PASS
177	176	5	9	5.9	3543	PASS

Scan 2890 (10.621 min): VU062559.D\data.ms

BFB052

m/z Abundance



m/z	Abundance
36.10	524.0
37.00	2983.0
38.00	2489.0
39.00	802.0
43.90	440.0
45.00	379.0
46.90	393.0
47.90	428.0
49.00	2880.0
50.00	11536.0
51.00	3192.0
51.90	143.0
55.00	180.0
55.90	976.0
56.90	1899.0
59.90	603.0
60.90	3652.0
62.00	3464.0
63.00	2403.0
64.00	325.0
64.90	115.0
66.70	179.0
68.00	6987.0
69.00	7740.0
70.00	585.0
71.90	318.0
73.00	3375.0
74.00	12930.0
75.00	40312.0
75.90	3303.0
77.10	417.0
77.90	284.0
78.90	2278.0
79.90	559.0
80.90	2215.0
81.90	491.0
86.90	2154.0
87.90	2579.0
90.90	256.0
92.00	2246.0
92.90	3202.0
94.00	9018.0
95.00	71536.0
96.00	4650.0
96.80	136.0
103.80	397.0
104.70	105.0
105.90	295.0
115.90	251.0
116.90	610.0
117.90	287.0
118.90	456.0
127.90	316.0
128.70	118.0
129.80	220.0
134.90	132.0
136.80	173.0
140.90	975.0
141.90	144.0
142.90	1091.0
145.80	120.0
147.60	180.0
154.80	168.0
156.90	198.0
160.90	139.0
171.70	180.0
173.90	57288.0
174.90	4176.0
175.90	55776.0
176.90	3272.0
177.80	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB052

m/z	Abundance
36.10	573.0
37.00	3096.0
38.00	2583.0
38.90	893.0
43.90	480.0
45.00	406.0
47.00	425.0
47.90	480.0
49.00	3113.0
50.00	12231.0
51.00	3427.0
51.90	137.0
55.00	163.0
56.00	993.0
56.90	1992.0
57.80	107.0
59.90	652.0
60.90	3866.0
62.00	3696.0
63.00	2584.0
64.00	372.0
64.90	167.0
67.00	157.0
68.00	7570.0
69.00	7780.0
70.00	588.0
72.00	379.0
73.00	3332.0
74.00	13766.0
75.00	43056.0
76.00	3461.0
77.10	398.0
78.00	289.0
78.90	2437.0
79.90	662.0
80.90	2403.0
81.90	432.0
87.00	2328.0
87.90	2701.0
90.90	307.0
92.00	2322.0
92.90	3476.0
94.00	9334.0
95.00	77720.0
96.00	4954.0
96.90	111.0
103.80	426.0
104.70	135.0
106.00	321.0
112.80	100.0
115.80	296.0
116.90	583.0
117.90	298.0
118.90	463.0
127.80	329.0
128.70	151.0
129.80	260.0
134.90	155.0
136.80	156.0
140.80	1227.0
141.90	159.0
142.90	1279.0
143.70	105.0
144.80	102.0
145.90	100.0
147.60	180.0
154.80	181.0
156.90	214.0
160.80	123.0
171.80	164.0
173.90	62336.0
174.90	4747.0
175.90	61360.0
176.80	3633.0
177.80	130.0

Instrument :
MSVOA_U
ClientSampleId :
BFB052

m/z	Abundance
36.00	532.0
37.00	2995.0
38.00	2419.0
38.90	852.0
43.90	410.0
45.00	437.0
47.10	456.0
47.90	446.0
49.00	2969.0
50.00	12174.0
51.00	3468.0
55.00	150.0
55.90	993.0
57.00	1934.0
59.90	611.0
61.00	3706.0
62.00	3472.0
63.00	2615.0
64.00	382.0
65.00	199.0
67.00	149.0
68.00	7416.0
69.00	7554.0
70.00	492.0
72.00	427.0
73.00	3120.0
74.00	13687.0
75.00	41880.0
76.00	3444.0
77.10	367.0
78.00	273.0
78.90	2312.0
79.90	704.0
80.90	2298.0
81.90	417.0
87.00	2267.0
87.90	2421.0
90.90	333.0
92.00	2265.0
92.90	3359.0
94.00	9053.0
95.00	76640.0
96.00	4989.0
97.00	111.0
103.80	356.0
104.80	144.0
106.00	336.0
115.80	299.0
116.90	562.0
117.90	253.0
118.90	441.0
127.80	309.0
128.80	161.0
129.90	305.0
130.90	107.0
134.90	143.0
136.80	133.0
140.80	1288.0
141.90	138.0
142.90	1259.0
143.70	114.0
144.80	127.0
145.70	112.0
147.60	154.0
149.70	124.0
154.80	183.0
156.90	183.0
171.90	146.0
173.90	61800.0
174.90	4867.0
175.90	61632.0
176.90	3723.0
177.80	131.0

Instrument :
MSVOA_U
ClientSampleId :
BFB052