


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122418\
 Data File : VU028931.D
 Acq On : 24 Dec 2018 08:26
 Operator : MD/SY
 Sample : BFB65
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB65

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
 Title : VOC Analysis
 Last Update : Tue Dec 25 00:02:36 2018

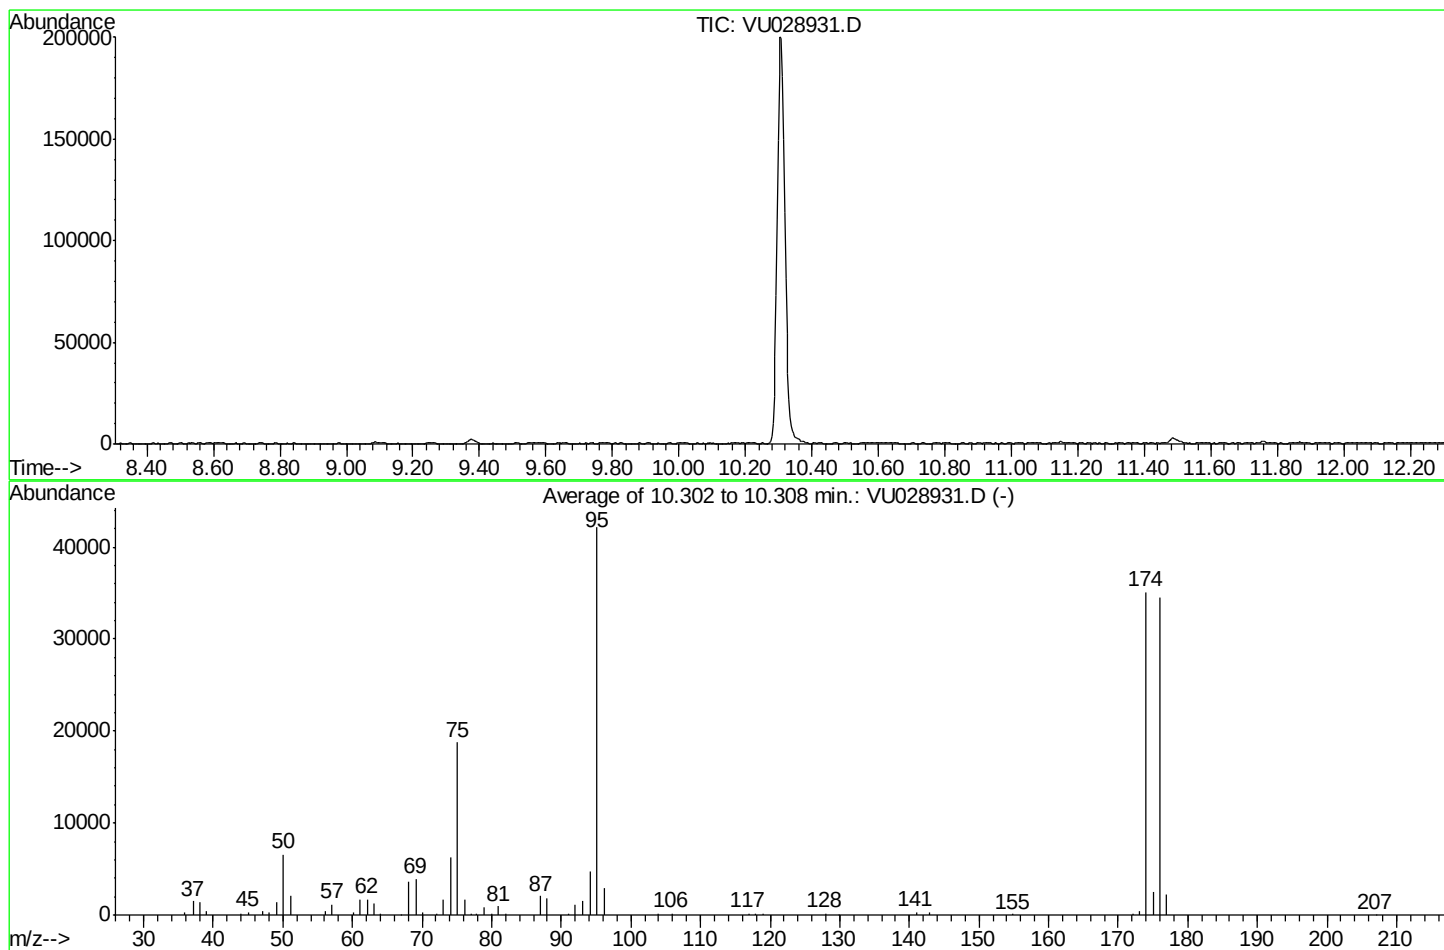

AutoFind: Scans 2839, 2840, 2841; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	6578	PASS
75	95	30	80	44.5	18741	PASS
95	95	100	100	100.0	42154	PASS
96	95	5	9	7.0	2954	PASS
173	174	0.00	2	1.2	408	PASS
174	95	50	120	83.3	35117	PASS
175	174	5	9	7.3	2548	PASS
176	174	95	101	98.5	34573	PASS
177	176	5	9	6.6	2271	PASS

m/z	Abundance
35.90	256.0
37.10	1464.0
38.10	1307.0
39.00	455.0
44.00	447.0
45.00	295.0
47.10	414.0
48.00	194.0
49.10	1394.0
50.10	6465.0
51.10	1986.0
56.10	441.0
57.10	1065.0
60.10	339.0
61.10	1527.0
62.10	1618.0
63.10	1201.0
64.00	144.0
68.10	3451.0
69.10	3808.0
70.00	258.0
72.10	161.0
73.00	1451.0
74.10	5827.0
75.10	17656.0
76.10	1647.0
77.10	220.0
77.80	190.0
79.00	785.0
80.00	152.0
81.00	955.0
82.00	167.0
87.00	2023.0
88.00	1687.0
91.00	111.0
92.00	982.0
93.00	1388.0
94.10	4560.0
95.10	39904.0
96.10	2774.0
104.00	133.0
105.90	168.0
116.90	149.0
117.80	123.0
119.00	116.0
128.00	106.0
141.00	332.0
142.90	254.0
172.00	124.0
173.00	394.0
174.00	32528.0
175.00	2408.0
176.00	31728.0
177.00	2132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB65

m/z	Abundance
44.00	247.0

Instrument :
MSVOA_U
ClientSampleId :
BFB65

m/z	Abundance
36.00	288.0
37.10	1478.0
38.10	1485.0
39.00	474.0
44.00	413.0
45.10	297.0
47.00	512.0
48.00	240.0
49.10	1430.0
50.10	6473.0
51.10	2130.0
56.00	496.0
57.10	1155.0
60.10	318.0
61.10	1723.0
62.10	1707.0
63.10	1173.0
64.00	198.0
67.00	100.0
68.10	3719.0
69.10	3964.0
70.10	221.0
72.10	203.0
73.10	1841.0
74.10	6394.0
75.10	19256.0
76.10	1669.0
77.10	192.0
77.90	210.0
78.90	825.0
80.00	174.0
81.00	891.0
81.90	171.0
87.00	2029.0
88.00	1990.0
90.90	125.0
92.00	1122.0
93.10	1528.0
94.10	4754.0
95.10	42896.0
96.10	3006.0
104.00	165.0
105.90	178.0
116.90	185.0
117.80	104.0
119.00	122.0
127.90	167.0
141.00	363.0
142.90	296.0
154.90	123.0
172.10	103.0
173.10	412.0
174.00	36648.0
175.00	2631.0
176.00	36312.0
177.00	2329.0
207.00	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB65

m/z	Abundance
36.00	273.0
37.10	1562.0
38.10	1424.0
39.00	503.0
44.00	456.0
45.00	286.0
47.00	484.0
48.00	230.0
49.10	1466.0
50.10	6797.0
51.10	2158.0
56.10	471.0
57.10	1201.0
60.10	339.0
61.10	1733.0
62.10	1731.0
63.10	1229.0
64.00	177.0
68.10	3763.0
69.10	4098.0
70.10	246.0
72.10	187.0
73.10	1713.0
74.10	6454.0
75.10	19312.0
76.10	1700.0
77.10	220.0
77.90	207.0
79.00	824.0
80.00	181.0
81.00	957.0
81.90	183.0
87.00	2135.0
88.00	1955.0
90.90	117.0
92.00	1116.0
93.00	1512.0
94.10	4919.0
95.10	43664.0
96.10	3083.0
104.00	164.0
105.90	193.0
116.90	181.0
117.80	121.0
119.00	120.0
127.90	149.0
129.80	103.0
141.00	365.0
142.90	279.0
154.90	115.0
172.10	118.0
173.10	419.0
174.00	36176.0
175.00	2607.0
176.00	35680.0
177.00	2354.0

Instrument :
MSVOA_U
ClientSampleId :
BFB65