


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU122420\
 Data File : VU041796.D
 Acq On : 24 Dec 2020 08:36
 Operator : SY/MD
 Sample : BFB32
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB202

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SFAMULM121620WMA.M
 Title : VOC Analysis
 Last Update : Fri Dec 25 02:17:32 2020

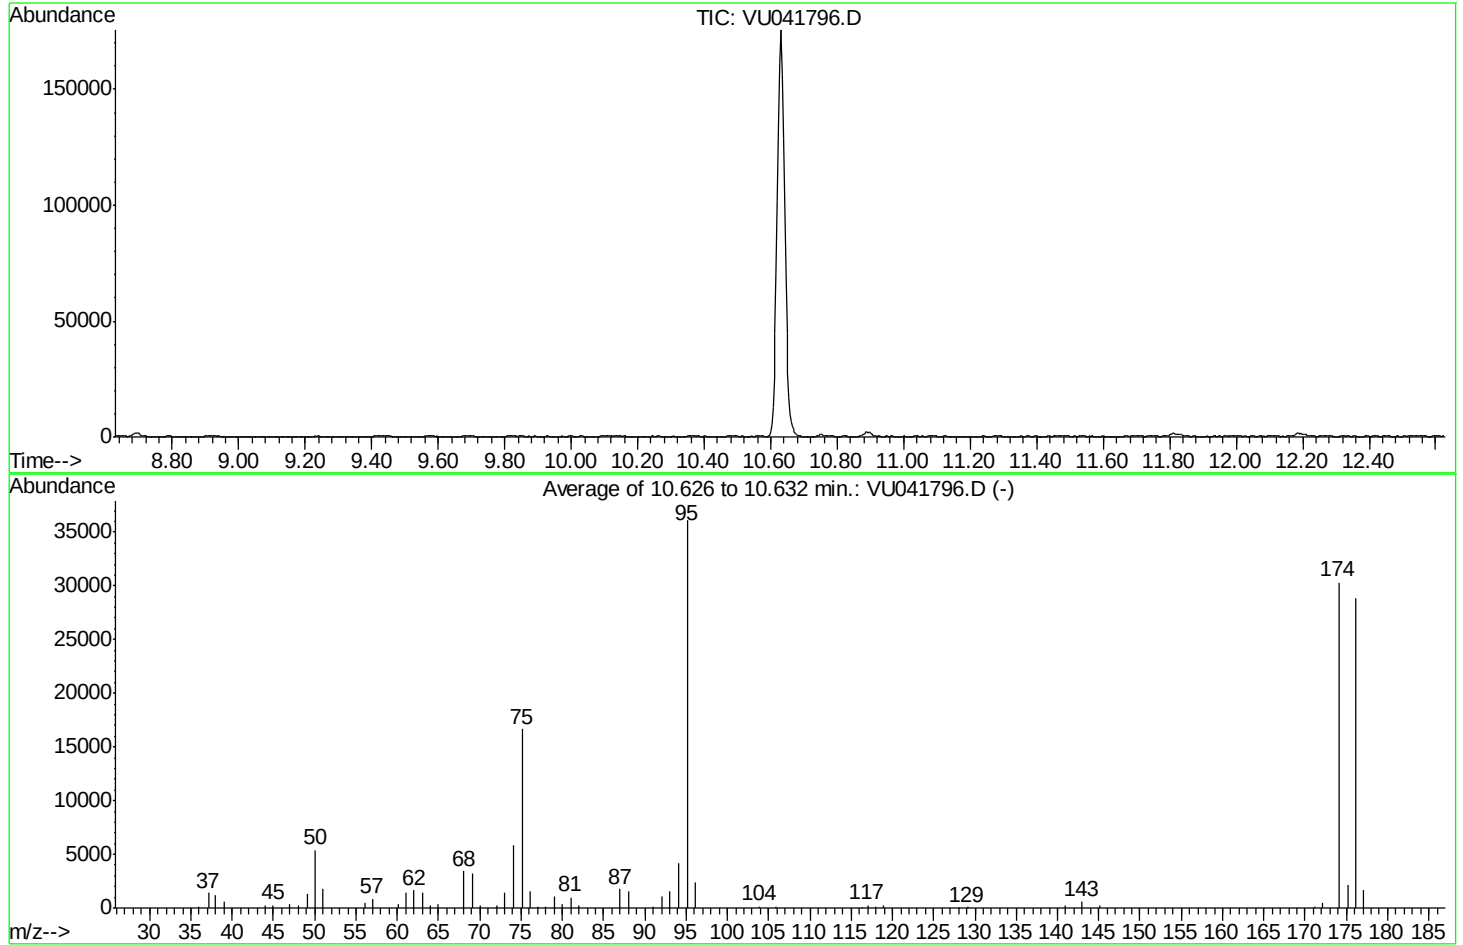

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.0	5421	PASS
75	95	30	80	46.1	16656	PASS
95	95	100	100	100.0	36093	PASS
96	95	5	9	6.5	2356	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.0	30309	PASS
175	174	5	9	7.2	2176	PASS
176	174	95	101	95.1	28818	PASS
177	176	5	9	5.8	1664	PASS

m/z	Abundance
35.90	165.0
37.10	1247.0
38.00	1069.0
39.00	602.0
44.00	337.0
45.00	267.0
47.00	367.0
48.00	185.0
49.10	1379.0
50.10	5258.0
51.00	1824.0
56.10	464.0
57.00	834.0
60.10	327.0
61.10	1279.0
62.10	1619.0
63.00	1352.0
64.00	269.0
65.00	331.0
68.00	3375.0
69.10	2897.0
70.10	243.0
72.20	172.0
73.00	1421.0
74.10	5277.0
75.10	16408.0
76.10	1485.0
77.10	116.0
79.00	1116.0
79.90	376.0
81.00	831.0
81.90	182.0
87.00	1745.0
88.00	1501.0
91.00	153.0
92.10	1050.0
93.00	1435.0
94.10	4138.0
95.10	34296.0
96.10	2355.0
103.90	175.0
105.90	121.0
116.20	145.0
117.00	262.0
117.90	101.0
118.90	212.0
140.90	228.0
143.00	549.0
145.10	265.0
171.10	117.0
172.10	421.0
174.10	28264.0
175.20	2194.0
176.10	26936.0
177.00	1579.0

Instrument :
MSVOA_U
ClientSampleId :
BFB202

m/z	Abundance
35.90	185.0
37.10	1475.0
38.00	1225.0
39.00	628.0
44.00	366.0
45.00	291.0
46.90	394.0
48.00	219.0
49.10	1405.0
50.00	5592.0
51.00	1899.0
56.10	465.0
57.00	898.0
60.00	324.0
61.10	1453.0
62.00	1700.0
63.00	1475.0
64.00	258.0
65.00	363.0
68.00	3633.0
69.10	3252.0
70.00	266.0
72.20	232.0
73.10	1555.0
74.10	6115.0
75.10	17072.0
76.10	1504.0
77.10	152.0
78.00	104.0
79.00	1150.0
80.00	430.0
81.00	1069.0
81.90	231.0
87.00	1898.0
88.00	1667.0
90.90	127.0
92.00	1079.0
93.00	1563.0
94.10	4413.0
95.10	37264.0
96.10	2458.0
103.90	186.0
105.80	121.0
117.00	288.0
118.00	135.0
119.00	262.0
129.10	109.0
140.90	240.0
143.00	599.0
145.10	259.0
171.10	148.0
172.10	559.0
174.10	31288.0
175.20	2205.0
176.10	29680.0
177.00	1703.0

Instrument :
MSVOA_U
ClientSampleId :
BFB202

m/z	Abundance
35.90	190.0
37.10	1506.0
38.00	1172.0
39.10	567.0
44.00	311.0
45.00	256.0
47.00	379.0
48.10	199.0
49.00	1235.0
50.00	5415.0
51.00	1748.0
56.00	407.0
57.00	828.0
60.00	323.0
61.10	1478.0
62.00	1629.0
63.00	1555.0
64.00	251.0
65.00	402.0
68.10	3315.0
69.10	3339.0
70.00	269.0
72.00	272.0
73.10	1501.0
74.10	6299.0
75.10	16488.0
76.10	1512.0
77.10	196.0
78.00	100.0
79.00	1130.0
80.00	416.0
81.00	1134.0
82.00	284.0
87.00	1673.0
88.10	1600.0
90.90	115.0
92.00	1080.0
93.00	1554.0
94.10	4140.0
95.10	36720.0
96.10	2255.0
103.90	157.0
117.00	255.0
118.00	158.0
119.00	286.0
128.00	120.0
129.10	147.0
140.90	258.0
143.00	624.0
145.10	237.0
171.10	134.0
172.10	591.0
174.10	31376.0
175.10	2131.0
176.10	29840.0
177.00	1712.0

Instrument :
MSVOA_U
ClientSampleId :
BFB202

m/z	Abundance
43.90	130.0

Instrument :
MSVOA_U
ClientSampleId :
BFB202