

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U122520\
 Data File : VU041806.D
 Acq On : 24 Dec 2020 15:06
 Operator : SY/MD
 Sample : L5161-12DL 2X
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GB237DL

Quant Time: Dec 25 04:13:56 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Fri Dec 25 03:47:04 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.26	114	134727	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.42	117	134313	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.81	152	61425	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.60	65	36060	3.42	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	68.40%
7) Chloroethane-d5	1.92	69	39717	4.87	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.40%
11) 1,1-Dichloroethene-d2	2.58	63	58852	3.03	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.60%
20) 2-Butanone-d5	4.66	46	166533	55.04	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.08%
24) Chloroform-d	5.08	84	82970	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.00%
26) 1,2-Dichloroethane-d4	5.72	65	49153	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.00%
32) Benzene-d6	5.74	84	153521	3.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	79.80%
36) 1,2-Dichloropropane-d6	6.70	67	51542	4.27	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	85.40%
41) Toluene-d8	7.90	98	124165	3.58	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.60%
43) trans-1,3-Dichloropropene-	8.19	79	20753	3.83	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.60%
46) 2-Hexanone-d5	8.64	63	131146	44.25	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.50%
57) 1,1,2,2-Tetrachloroethane-	10.75	84	46186	4.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.40%
64) 1,2-Dichlorobenzene-d4	12.19	152	49245	4.51	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	90.20%


Target Compounds					Ovalue
31) Carbon tetrachloride	5.54	117	121940	9.143 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU122520\
Data File : VU041806.D
Acq On : 24 Dec 2020 15:06
Operator : SY/MD
Sample : L5161-12DL 2X
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GB237DL

Quant Time: Dec 25 04:13:56 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Dec 25 03:47:04 2020
Response via : Initial Calibration

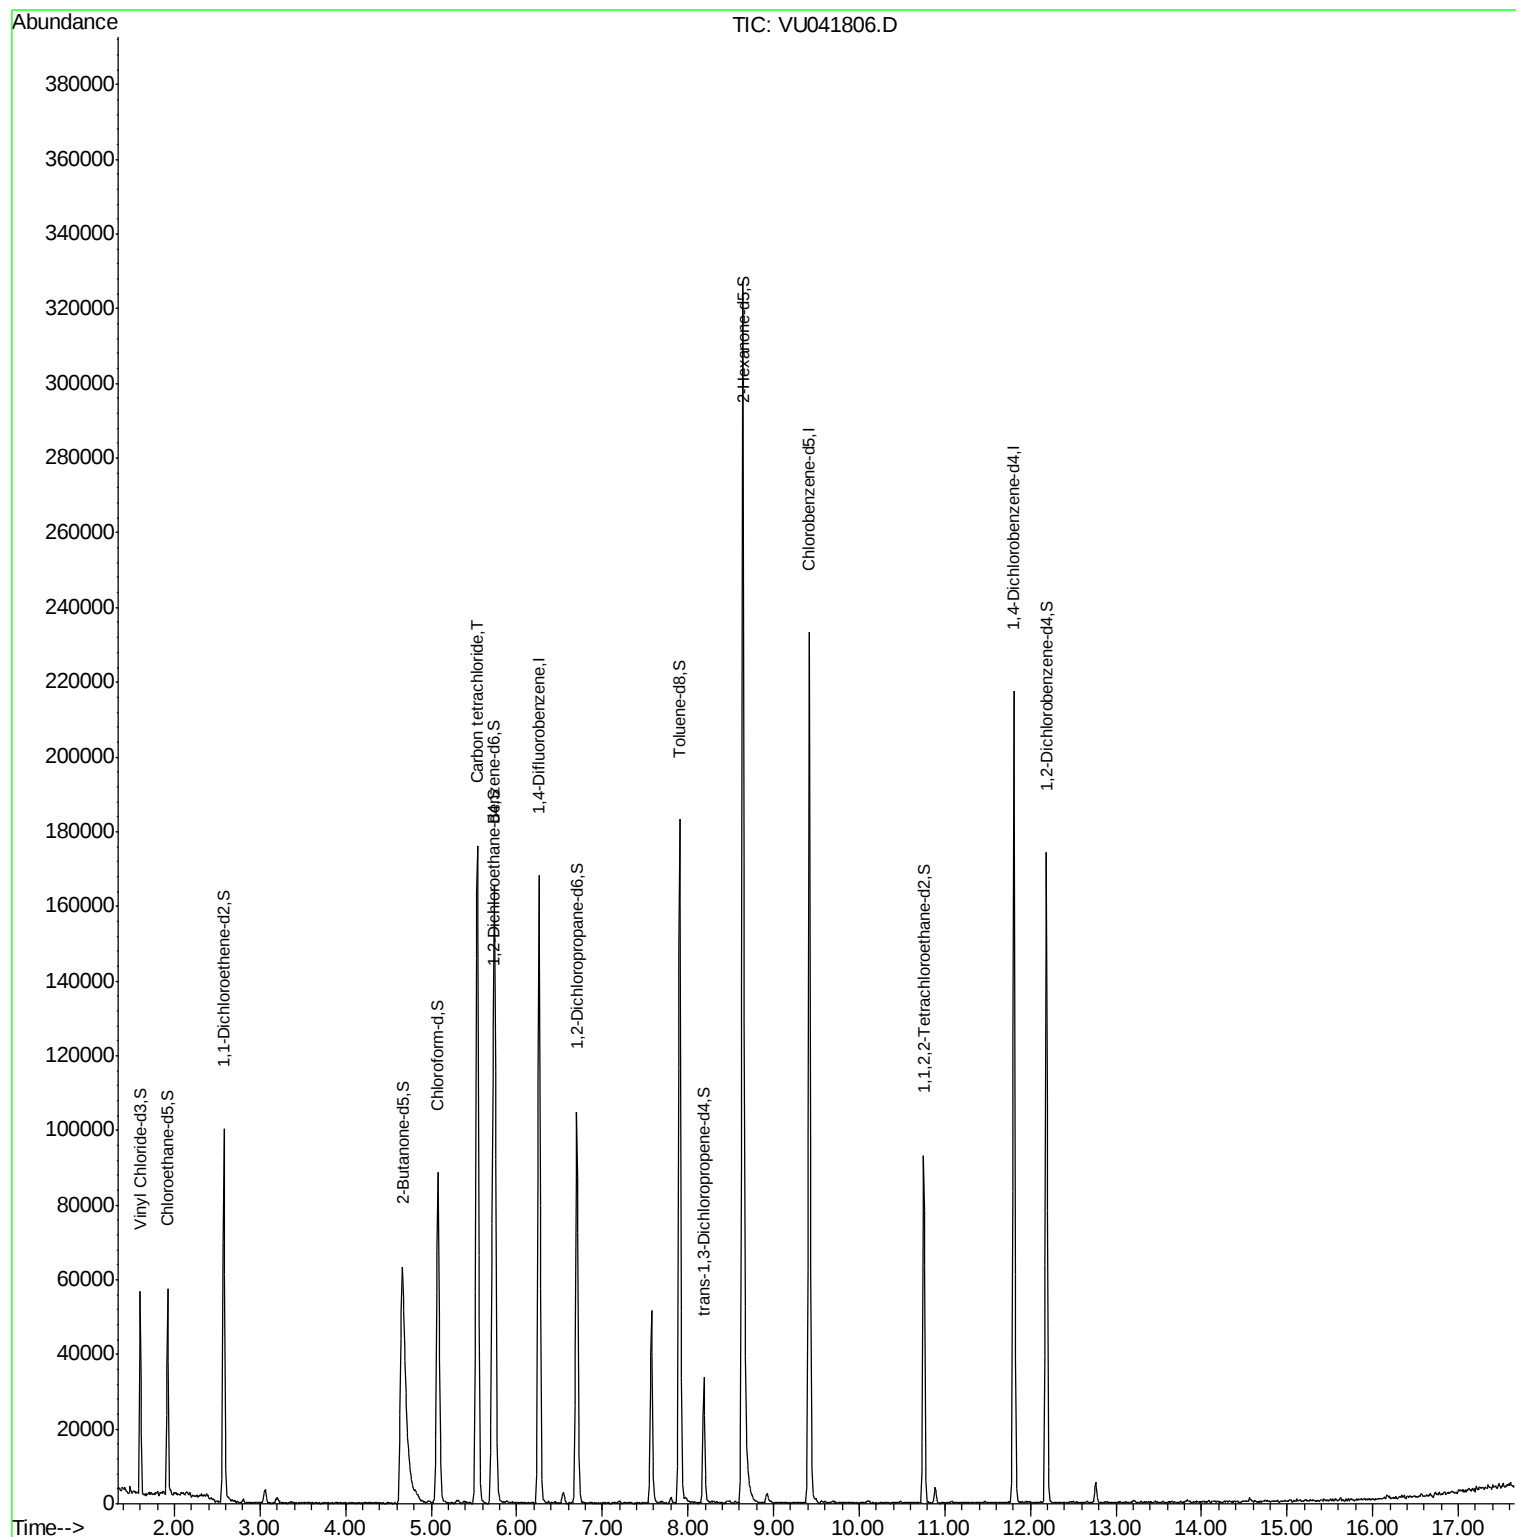

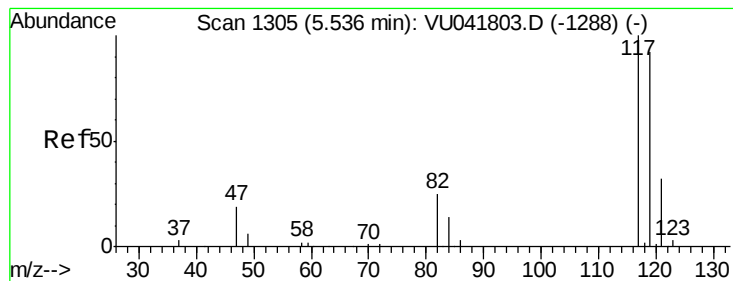

#31

Carbon tetrachloride

Concen: 9.143 ug/L

RT: 5.54 min Scan# 1306

Delta R.T. 0.00 min

Lab File: VU041806.D

Acq: 24 Dec 2020 15:06

Instrument :

MSVOA_U

ClientSampleId :

GB237DL

Tot Ion:117 Resp: 121940

Ion Ratio Lower Upper

117 100

119 97.9 76.2 114.2

