


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU122520\
 Data File : VU041802.D
 Acq On : 24 Dec 2020 12:28
 Operator : SY/MD
 Sample : BFB30
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB30

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121220WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Fri Dec 25 03:47:04 2020

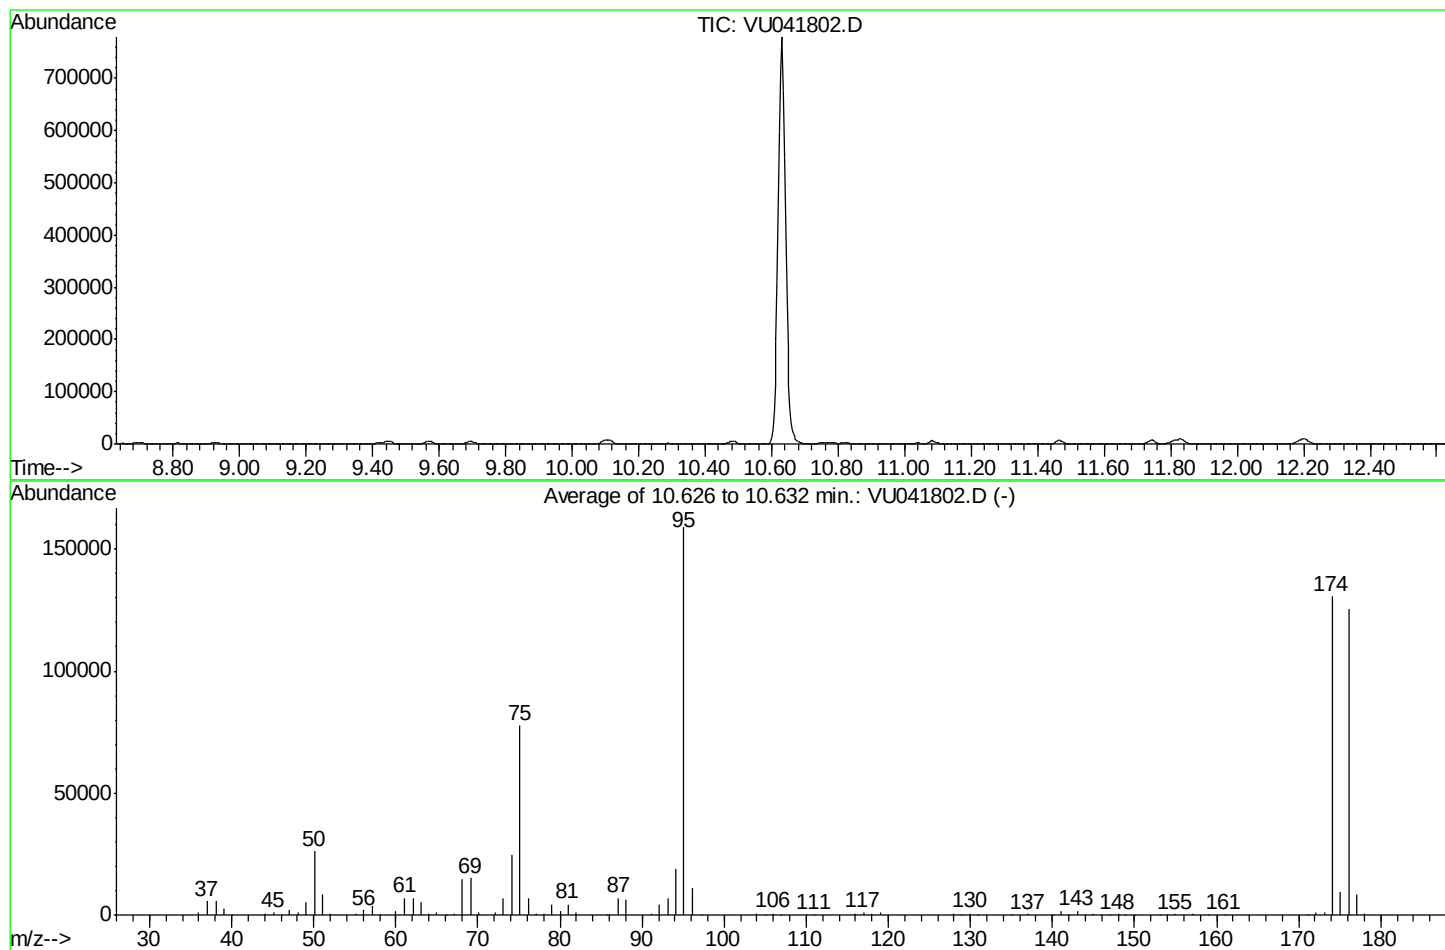

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	26072	PASS
75	95	30	80	48.8	77512	PASS
95	95	100	100	100.0	158976	PASS
96	95	5	9	6.9	10890	PASS
173	174	0.00	2	1.0	1280	PASS
174	95	50	120	82.2	130680	PASS
175	174	5	9	7.4	9622	PASS
176	174	95	101	96.0	125506	PASS
177	176	5	9	6.7	8398	PASS

m/z	Abundance
35.90	995.0
37.00	5734.0
38.10	5492.0
39.00	2390.0
40.10	174.0
44.00	768.0
45.10	987.0
46.00	126.0
47.00	1892.0
48.10	867.0
49.10	5361.0
50.10	25864.0
51.10	8596.0
52.00	398.0
55.10	330.0
56.10	2015.0
57.10	3771.0
58.00	137.0
60.00	1410.0
61.10	6850.0
62.10	6972.0
63.10	5293.0
64.00	765.0
65.00	958.0
66.20	203.0
67.10	423.0
68.10	14632.0
69.10	14110.0
70.00	1103.0
72.10	855.0
73.10	6417.0
74.10	23920.0
75.10	74416.0
76.10	6722.0
77.10	777.0
78.00	589.0
79.00	4285.0
80.10	1451.0
81.00	4132.0
82.00	937.0
85.70	134.0
87.10	6613.0
88.00	5919.0
91.10	569.0
92.10	4091.0
93.10	6837.0
94.10	17752.0
95.10	151808.0
96.10	10779.0
97.20	180.0
104.00	558.0
105.00	236.0
106.00	483.0
106.90	173.0
111.00	133.0
116.00	480.0
117.00	999.0
118.00	580.0
119.00	906.0
128.00	436.0
128.90	230.0
130.00	522.0
130.90	182.0
134.90	276.0
137.00	285.0
141.10	1387.0
142.00	162.0
143.10	1649.0
145.00	544.0
145.90	174.0
147.00	100.0
148.00	396.0
150.10	171.0
154.00	119.0
155.00	350.0
157.10	301.0
159.10	159.0
161.00	166.0
171.20	143.0
172.10	1120.0
174.10	122728.0
175.10	9150.0
176.10	116648.0
177.10	7998.0
178.00	264.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30

m/z	Abundance
35.00	1021.0
37.00	5709.0
38.10	5754.0
39.00	2555.0
40.10	191.0
44.10	806.0
45.10	1031.0
47.00	1937.0
48.10	1022.0
49.10	5617.0
50.10	27072.0
51.10	9012.0
52.00	454.0
55.10	326.0
56.10	2145.0
57.10	3954.0
58.00	177.0
60.00	1513.0
61.10	7347.0
62.10	7267.0
63.10	5362.0
64.10	774.0
65.00	1030.0
66.20	212.0
67.00	468.0
68.10	15087.0
69.10	15689.0
70.10	1244.0
72.10	854.0
73.10	7162.0
74.10	25424.0
75.10	80416.0
76.10	6922.0
77.00	793.0
78.00	648.0
79.00	4619.0
80.00	1565.0
81.00	4447.0
82.00	1007.0
87.10	7191.0
88.00	6199.0
91.10	608.0
92.10	4470.0
93.10	7128.0
94.10	19544.0
95.10	164288.0
96.10	11256.0
97.20	221.0
104.00	505.0
105.00	219.0
106.00	588.0
106.90	158.0
110.00	147.0
111.00	162.0
116.00	533.0
117.00	1033.0
118.00	660.0
119.00	947.0
128.00	533.0
128.90	253.0
130.00	585.0
130.90	201.0
134.90	275.0
137.00	318.0
140.10	125.0
141.10	1421.0
142.00	228.0
143.10	1821.0
144.00	119.0
145.00	489.0
145.90	205.0
148.00	403.0
148.90	105.0
150.00	124.0
153.10	129.0
154.00	123.0
155.00	353.0
157.00	334.0
159.00	165.0
161.00	197.0
171.20	169.0
172.10	1261.0
173.20	1861.0
174.10	134656.0
175.10	9769.0
176.10	129640.0
177.10	8720.0
178.00	327.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30

m/z	Abundance
36.00	911.0
37.00	5395.0
38.00	5539.0
39.10	2509.0
40.00	147.0
44.10	819.0
45.10	958.0
46.00	105.0
47.00	1820.0
48.10	928.0
49.10	5278.0
50.10	25280.0
51.10	8319.0
52.00	436.0
55.10	348.0
56.10	2104.0
57.10	3666.0
58.00	180.0
60.00	1351.0
61.10	7065.0
62.10	6793.0
63.00	5193.0
64.10	720.0
65.00	1070.0
66.10	177.0
67.00	454.0
68.10	14273.0
69.10	15564.0
70.10	1246.0
72.10	736.0
73.10	7007.0
74.10	24112.0
75.10	77704.0
76.10	6462.0
77.00	750.0
78.00	615.0
79.00	4377.0
80.00	1370.0
81.00	4379.0
82.00	994.0
86.00	238.0
87.10	6877.0
88.10	6127.0
91.10	587.0
92.10	4366.0
93.10	6640.0
94.10	19016.0
95.10	160832.0
96.10	10636.0
97.20	266.0
104.00	503.0
105.00	194.0
106.00	668.0
106.80	125.0
110.00	159.0
111.00	150.0
116.00	549.0
117.00	1037.0
118.00	679.0
119.00	873.0
128.00	590.0
128.90	254.0
130.00	596.0
130.90	187.0
134.90	226.0
137.00	254.0
140.10	114.0
141.10	1274.0
141.90	257.0
143.00	1691.0
144.00	157.0
145.00	416.0
146.00	190.0
148.00	348.0
148.90	101.0
153.10	146.0
154.00	118.0
155.00	321.0
157.00	337.0
159.00	134.0
161.00	186.0
171.20	162.0
172.10	1169.0
173.20	1980.0
174.10	134656.0
175.10	9948.0
176.10	130232.0
177.10	8478.0
178.00	288.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30

m/z	Abundance
43.90	252.0

Instrument :
MSVOA_U
ClientSampleId :
BFB30