


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU122619\
Data File : VU036343.D
Acq On : 26 Dec 2019 09:37
Operator : JC/MD
Sample : BFB25
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB25

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR121319WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Dec 26 15:41:25 2019

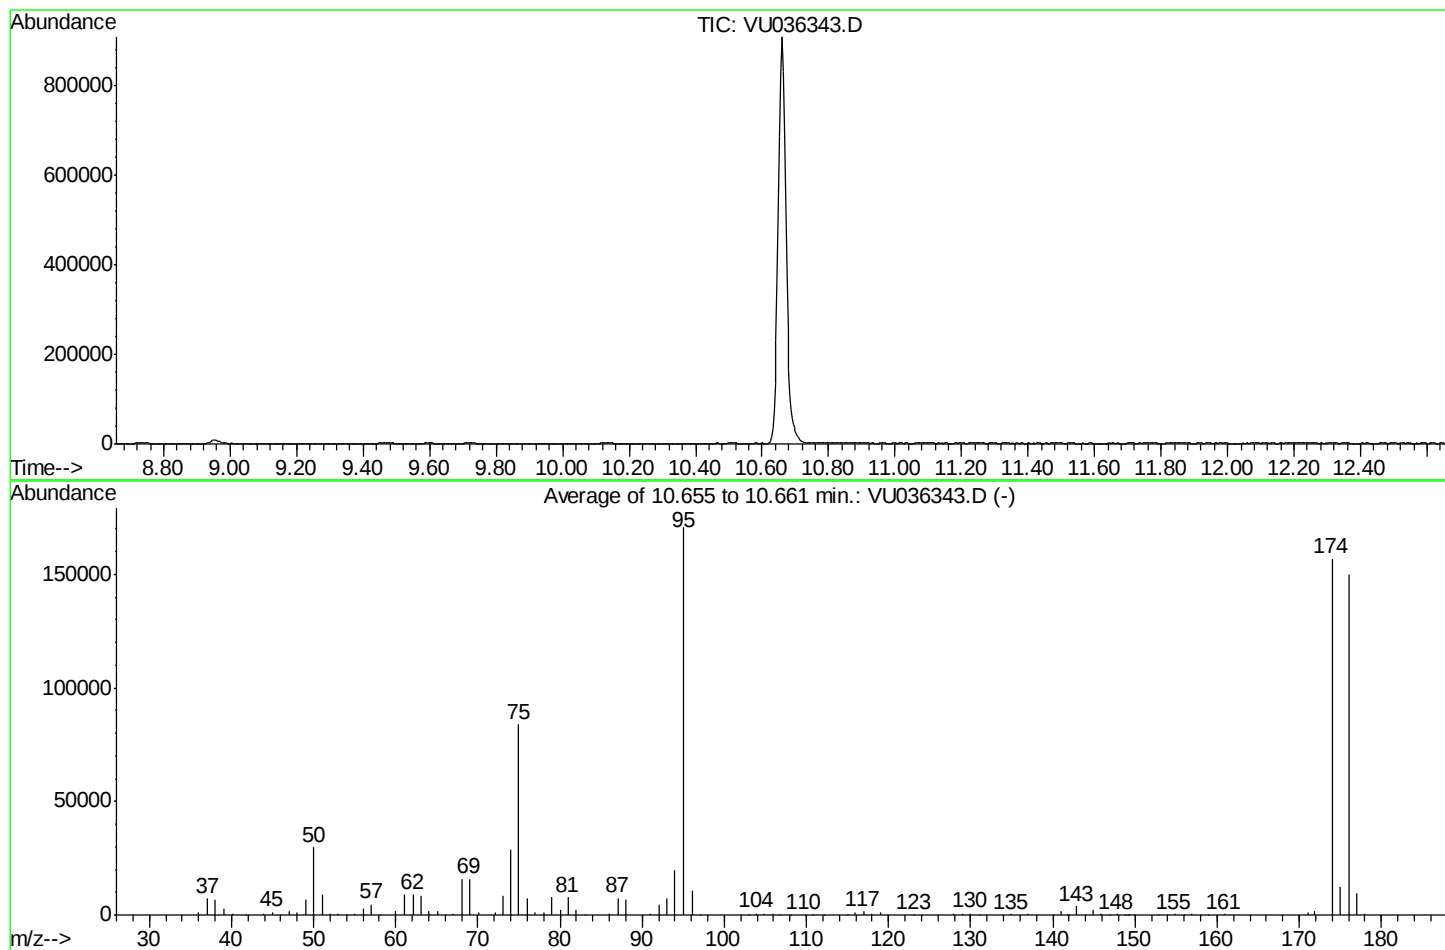

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	29813	PASS
75	95	30	80	49.1	83816	PASS
95	95	100	100	100.0	170666	PASS
96	95	5	9	6.3	10697	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	92.0	156928	PASS
175	174	5	9	7.9	12331	PASS
176	174	95	101	95.7	150122	PASS
177	176	5	9	6.5	9764	PASS

m/z	Abundance
36.00	1632.0
37.10	6857.0
38.00	7122.0
39.10	2545.0
40.20	400.0
41.70	118.0
43.90	1305.0
45.00	1057.0
46.10	337.0
47.00	1824.0
47.90	942.0
49.10	6527.0
50.10	28488.0
51.00	8680.0
52.00	346.0
52.90	499.0
54.10	156.0
55.10	284.0
56.10	2611.0
57.00	4758.0
58.10	182.0
60.00	1768.0
61.00	8403.0
62.10	8903.0
63.00	7929.0
64.00	1905.0
65.10	1534.0
66.10	172.0
67.10	528.0
68.00	15484.0
69.00	14902.0
70.10	1221.0
72.20	724.0
73.00	8463.0
74.00	27288.0
75.00	78520.0
76.00	6770.0
77.00	1247.0
78.00	834.0
78.90	7526.0
80.00	2315.0
81.00	7268.0
82.00	2326.0
83.00	209.0
86.00	378.0
87.00	7093.0
88.00	6121.0
91.00	641.0
92.00	4022.0
93.00	7045.0
94.00	18832.0
95.10	161728.0
96.10	10223.0
97.10	318.0
102.90	139.0
103.90	801.0
104.90	288.0
106.00	653.0
106.70	109.0
108.10	161.0
109.80	198.0
110.80	146.0
114.90	194.0
115.90	895.0
117.00	1681.0
118.00	772.0
118.90	1490.0
123.10	131.0
124.00	108.0
127.90	568.0
128.90	325.0
129.90	422.0
131.00	313.0
135.10	374.0
136.90	314.0
140.00	151.0
140.90	1568.0
141.80	235.0
142.90	3312.0
144.10	253.0
145.00	2155.0
145.90	323.0
147.00	202.0
147.80	369.0
149.10	119.0
149.80	228.0
153.00	195.0
153.90	126.0
154.80	382.0
156.00	156.0
156.80	245.0
159.00	191.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

160.90	232.0
171.00	965.0
171.90	1657.0
174.00	144704.0
175.00	11485.0
176.00	137920.0
176.90	9311.0
177.90	428.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
36.00	1790.0
37.10	7482.0
38.00	7325.0
39.10	2847.0
40.20	413.0
44.00	1412.0
45.00	1140.0
46.00	280.0
47.10	1975.0
47.90	1023.0
49.10	7118.0
50.00	30808.0
51.10	9032.0
52.10	378.0
52.90	478.0
54.10	287.0
55.10	325.0
56.10	2737.0
57.00	4835.0
58.10	203.0
60.00	1916.0
61.00	9143.0
62.10	9108.0
63.10	8760.0
64.00	2031.0
65.10	1673.0
66.00	185.0
67.00	681.0
68.00	16091.0
69.00	16266.0
70.00	1258.0
72.20	899.0
73.00	8854.0
74.00	29592.0
75.00	86552.0
76.10	7579.0
77.00	1295.0
78.00	969.0
78.90	8258.0
80.00	2366.0
81.00	8030.0
82.00	2307.0
83.00	196.0
86.00	370.0
87.00	7898.0
88.00	6845.0
91.00	745.0
92.00	4502.0
93.00	7730.0
94.00	20528.0
95.10	175488.0
96.10	10967.0
97.00	295.0
103.00	140.0
103.90	846.0
104.90	372.0
106.00	762.0
106.70	130.0
108.10	218.0
109.80	230.0
110.80	117.0
112.10	169.0
114.90	204.0
116.00	922.0
117.00	1714.0
118.00	756.0
118.90	1470.0
123.10	158.0
128.00	566.0
128.90	364.0
130.00	588.0
131.00	292.0
134.90	378.0
136.90	373.0
140.00	122.0
141.00	1761.0
141.80	221.0
142.90	3793.0
144.00	208.0
144.90	2164.0
145.90	361.0
147.00	184.0
147.80	487.0
148.80	115.0
149.10	114.0
149.80	233.0
152.90	182.0
153.90	111.0
154.80	428.0
156.00	181.0
156.90	350.0
159.00	246.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

160.90	335.0
171.00	1108.0
171.90	1976.0
174.00	161472.0
175.00	12698.0
176.00	155008.0
177.00	10075.0
177.90	338.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

m/z	Abundance
36.00	1702.0
37.10	7551.0
38.00	6693.0
39.10	2821.0
39.80	375.0
40.20	349.0
44.00	1425.0
45.00	1192.0
45.90	239.0
47.10	1741.0
47.90	994.0
49.00	6987.0
50.00	30144.0
51.10	9071.0
52.10	411.0
52.90	361.0
54.00	355.0
55.00	335.0
56.10	2541.0
57.10	4503.0
58.10	180.0
60.00	1897.0
61.00	8823.0
62.10	8608.0
63.10	8567.0
64.00	1883.0
65.10	1759.0
66.00	178.0
67.10	657.0
68.00	15810.0
69.00	16480.0
70.00	1115.0
72.10	1081.0
73.00	8259.0
74.00	29808.0
75.00	86376.0
76.10	7990.0
77.00	1194.0
78.00	873.0
78.90	8100.0
80.00	2263.0
81.00	8126.0
82.00	2167.0
83.00	183.0
86.00	304.0
87.00	7651.0
88.00	7121.0
91.00	793.0
92.00	4585.0
93.00	7978.0
94.00	20704.0
95.10	174784.0
96.10	10903.0
97.10	260.0
103.00	107.0
104.00	846.0
104.90	417.0
106.00	841.0
106.80	128.0
108.00	198.0
109.80	202.0
110.70	105.0
112.10	239.0
114.90	216.0
116.00	851.0
117.00	1622.0
118.00	794.0
119.00	1293.0
128.00	576.0
129.00	347.0
130.00	752.0
130.90	205.0
134.90	385.0
136.90	360.0
140.00	110.0
141.00	1770.0
142.00	235.0
142.90	4104.0
143.90	162.0
144.90	2008.0
145.90	322.0
146.80	151.0
147.80	561.0
149.30	118.0
149.90	231.0
152.80	191.0
154.80	494.0
156.00	143.0
156.90	355.0
158.00	101.0
158.90	213.0
160.90	374.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

171.00	1142.0
171.90	2259.0
174.00	164608.0
175.00	12811.0
176.00	157440.0
177.00	9907.0
177.90	277.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25

Scan 2883 (10.610 min): VU036343.D
BFB25

m/z	Abundance
36.00	281.0
37.90	178.0
40.00	156.0
43.90	529.0

Instrument :
MSVOA_U
ClientSampleId :
BFB25