




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122623\
 Data File : VU057257.D
 Acq On : 27 Dec 2023 02:07
 Operator : MD/SY
 Sample : 06002-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AG1

Manual IntegrationsAPPROVED

Quant Time: Dec 27 05:47:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 27 01:05:12 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 12/29/2023
 Supervised By :Mahesh Dadoda 12/29/2023

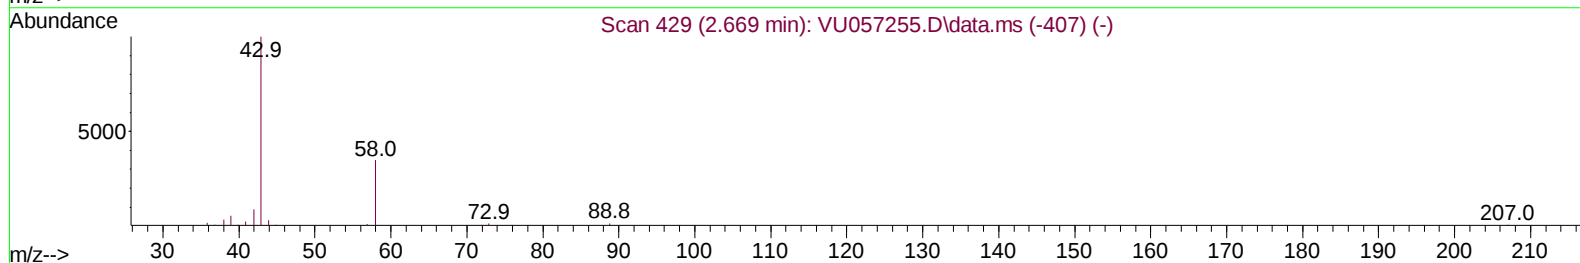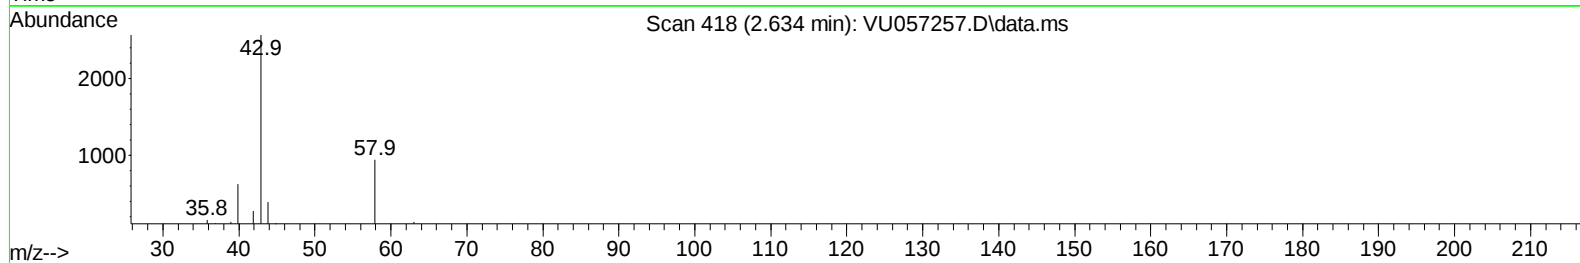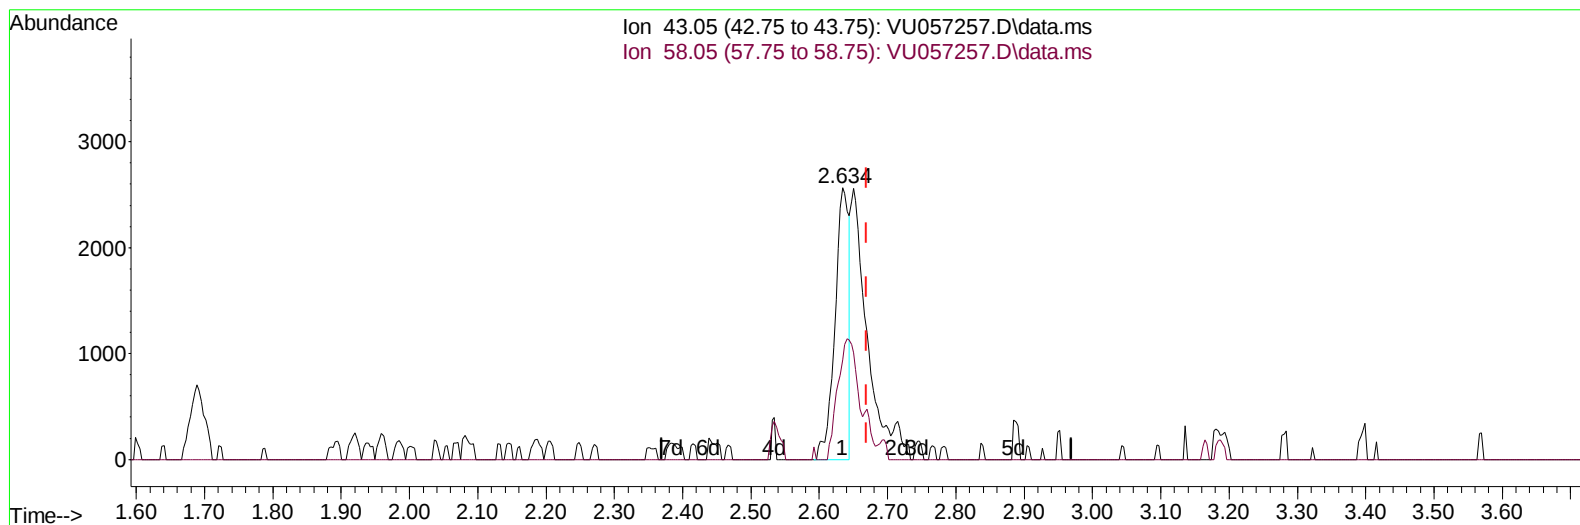

TIC: VU057257.D\data.ms

(13) Acetone (T)

2.634min (-0.035) 2.79 ug/L

response 3644

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.40	62.18
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122623\
 Data File : VU057257.D
 Acq On : 27 Dec 2023 02:07
 Operator : MD/SY
 Sample : 06002-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AG1

Manual IntegrationsAPPROVED

Quant Time: Dec 27 05:47:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 27 01:05:12 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 12/29/2023
 Supervised By :Mahesh Dadoda 12/29/2023

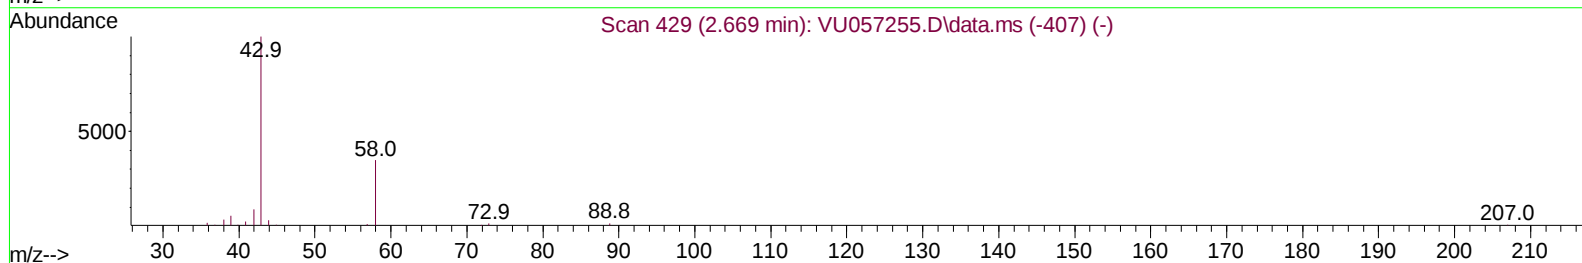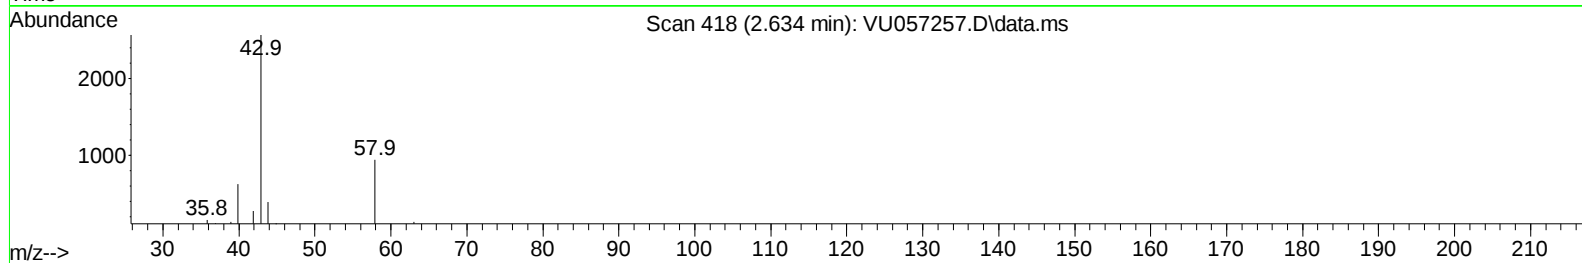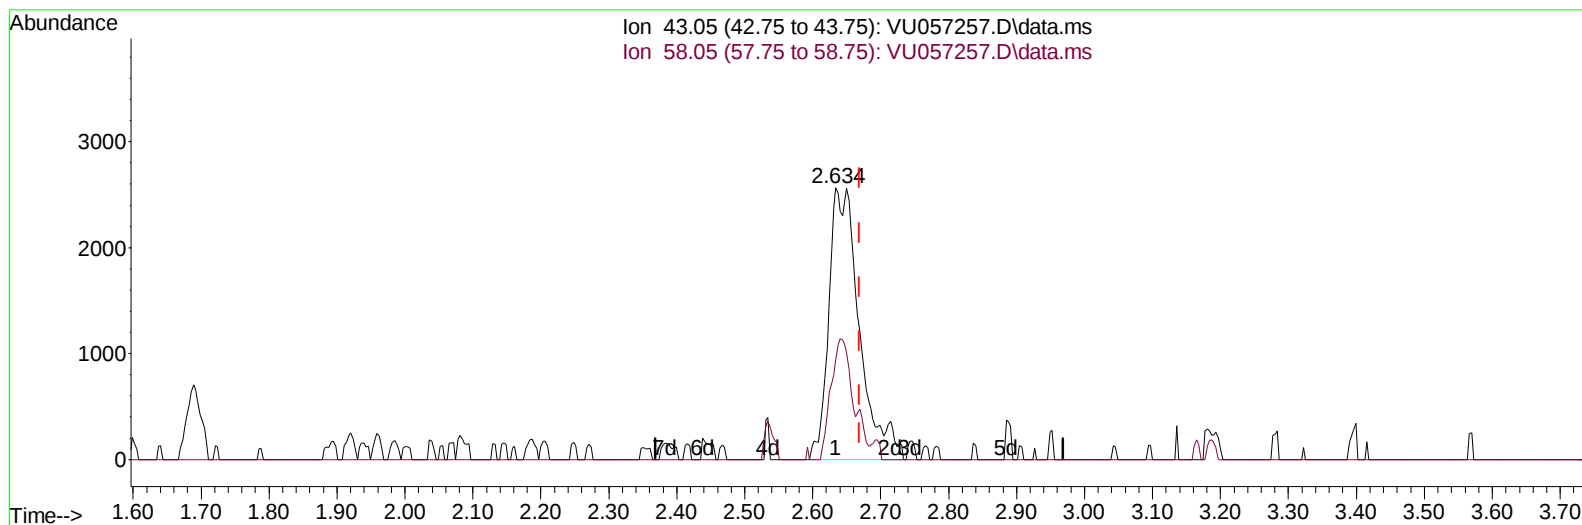

TIC: VU057257.D\data.ms

(13) Acetone (T)

2.634min (-0.035) 6.16 ug/L m

response 8038

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.40	28.19
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122623\
 Data File : VU057257.D
 Acq On : 27 Dec 2023 02:07
 Operator : MD/SY
 Sample : 06002-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AG1

Manual IntegrationsAPPROVED

Quant Time: Dec 27 05:47:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 27 01:05:12 2023
 Response via : Initial Calibration

Reviewed By : John Carlone 12/29/2023
 Supervised By : Mahesh Dadoda 12/29/2023

Compound		R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards								
1) 1,4-Difluorobenzene		6.245	114		144631	5.000	ug/L	0.00
28) Chlorobenzene-d5		9.415	117		151383	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		11.807	152		67251	5.000	ug/L	0.00
System Monitoring Compounds								
4) Vinyl Chloride-d3		1.599	65		89890	6.503	ug/L	0.00
Spiked Amount	5.000	Range	40	- 130	Recovery	=	130.000%	
7) Chloroethane-d5		1.914	69		66235	5.821	ug/L	0.00
Spiked Amount	5.000	Range	65	- 130	Recovery	=	116.400%	
11) 1,1-Dichloroethene-d2		2.563	65		34207	5.711	ug/L	0.00
Spiked Amount	5.000	Range	60	- 125	Recovery	=	114.200%	
20) 2-Butanone-d5		4.624	46		139717	64.372	ug/L	-0.02
Spiked Amount	50.000	Range	40	- 130	Recovery	=	128.740%	
24) Chloroform-d		5.055	84		145892	5.465	ug/L	0.00
Spiked Amount	5.000	Range	70	- 125	Recovery	=	109.200%	
26) 1,2-Dichloroethane-d4		5.698	65		69524	5.464	ug/L	0.00
Spiked Amount	5.000	Range	70	- 130	Recovery	=	109.200%	
32) Benzene-d6		5.721	84		267443	5.151	ug/L	0.00
Spiked Amount	5.000	Range	70	- 125	Recovery	=	103.000%	
36) 1,2-Dichloropropane-d6		6.685	67		82153	5.560	ug/L	0.00
Spiked Amount	5.000	Range	60	- 140	Recovery	=	111.200%	
41) Toluene-d8		7.894	98		217387	4.586	ug/L	0.00
Spiked Amount	5.000	Range	70	- 130	Recovery	=	91.800%	
43) trans-1,3-Dichloroprop...		8.177	79		30110	4.895	ug/L	0.00
Spiked Amount	5.000	Range	55	- 130	Recovery	=	98.000%	
46) 2-Hexanone-d5		8.631	63		105786	50.515	ug/L	0.00
Spiked Amount	50.000	Range	45	- 130	Recovery	=	101.020%	
56) 1,1,2,2-Tetrachloroeth...		10.753	84		60034	5.710	ug/L	0.00
Spiked Amount	5.000	Range	65	- 120	Recovery	=	114.200%	
66) 1,2-Dichlorobenzene-d4		12.190	152		72763	5.028	ug/L	0.00
Spiked Amount	5.000	Range	80	- 120	Recovery	=	100.600%	
Target Compounds								
13) Acetone		2.634	43		8038m	6.160	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122623\
Data File : VU057257.D
Acq On : 27 Dec 2023 02:07
Operator : MD/SY
Sample : 06002-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AG1

Manual IntegrationsAPPROVED

Quant Time: Dec 27 05:47:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Dec 27 01:05:12 2023
Response via : Initial Calibration

Reviewed By :John Carlone 12/29/2023
Supervised By :Mahesh Dadoda 12/29/2023

