

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122623\
 Data File : VU057257.D
 Acq On : 27 Dec 2023 02:07
 Operator : MD/SY
 Sample : 06002-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AG1

Manual Integrations
 APPROVED

Reviewed By : John Carlone 12/29/2023
 Supervised By : Mahesh Dadoda 12/29/2023

Quant Time: Dec 27 05:47:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 27 01:05:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	144631	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.415	117	151383	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	67251	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.599	65	89890	6.503	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery = 130.000%			
7) Chloroethane-d5	1.914	69	66235	5.821	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery = 116.400%			
11) 1,1-Dichloroethene-d2	2.563	65	34207	5.711	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery = 114.200%			
20) 2-Butanone-d5	4.624	46	139717	64.372	ug/L	-0.02
Spiked Amount 50.000	Range 40 - 130		Recovery = 128.740%			
24) Chloroform-d	5.055	84	145892	5.465	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 109.200%			
26) 1,2-Dichloroethane-d4	5.698	65	69524	5.464	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 109.200%			
32) Benzene-d6	5.721	84	267443	5.151	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery = 103.000%			
36) 1,2-Dichloropropane-d6	6.685	67	82153	5.560	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery = 111.200%			
41) Toluene-d8	7.894	98	217387	4.586	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery = 91.800%			
43) trans-1,3-Dichloroprop...	8.177	79	30110	4.895	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery = 98.000%			
46) 2-Hexanone-d5	8.631	63	105786	50.515	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery = 101.020%			
56) 1,1,2,2-Tetrachloroeth...	10.753	84	60034	5.710	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery = 114.200%			
66) 1,2-Dichlorobenzene-d4	12.190	152	72763	5.028	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery = 100.600%			
Target Compounds						Qvalue
13) Acetone	2.634	43	8038m	6.160	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122623\
Data File : VU057257.D
Acq On : 27 Dec 2023 02:07
Operator : MD/SY
Sample : 06002-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
C0AG1

Quant Time: Dec 27 05:47:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Dec 27 01:05:12 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :John Carlone 12/29/2023
Supervised By :Mahesh Dadoda 12/29/2023

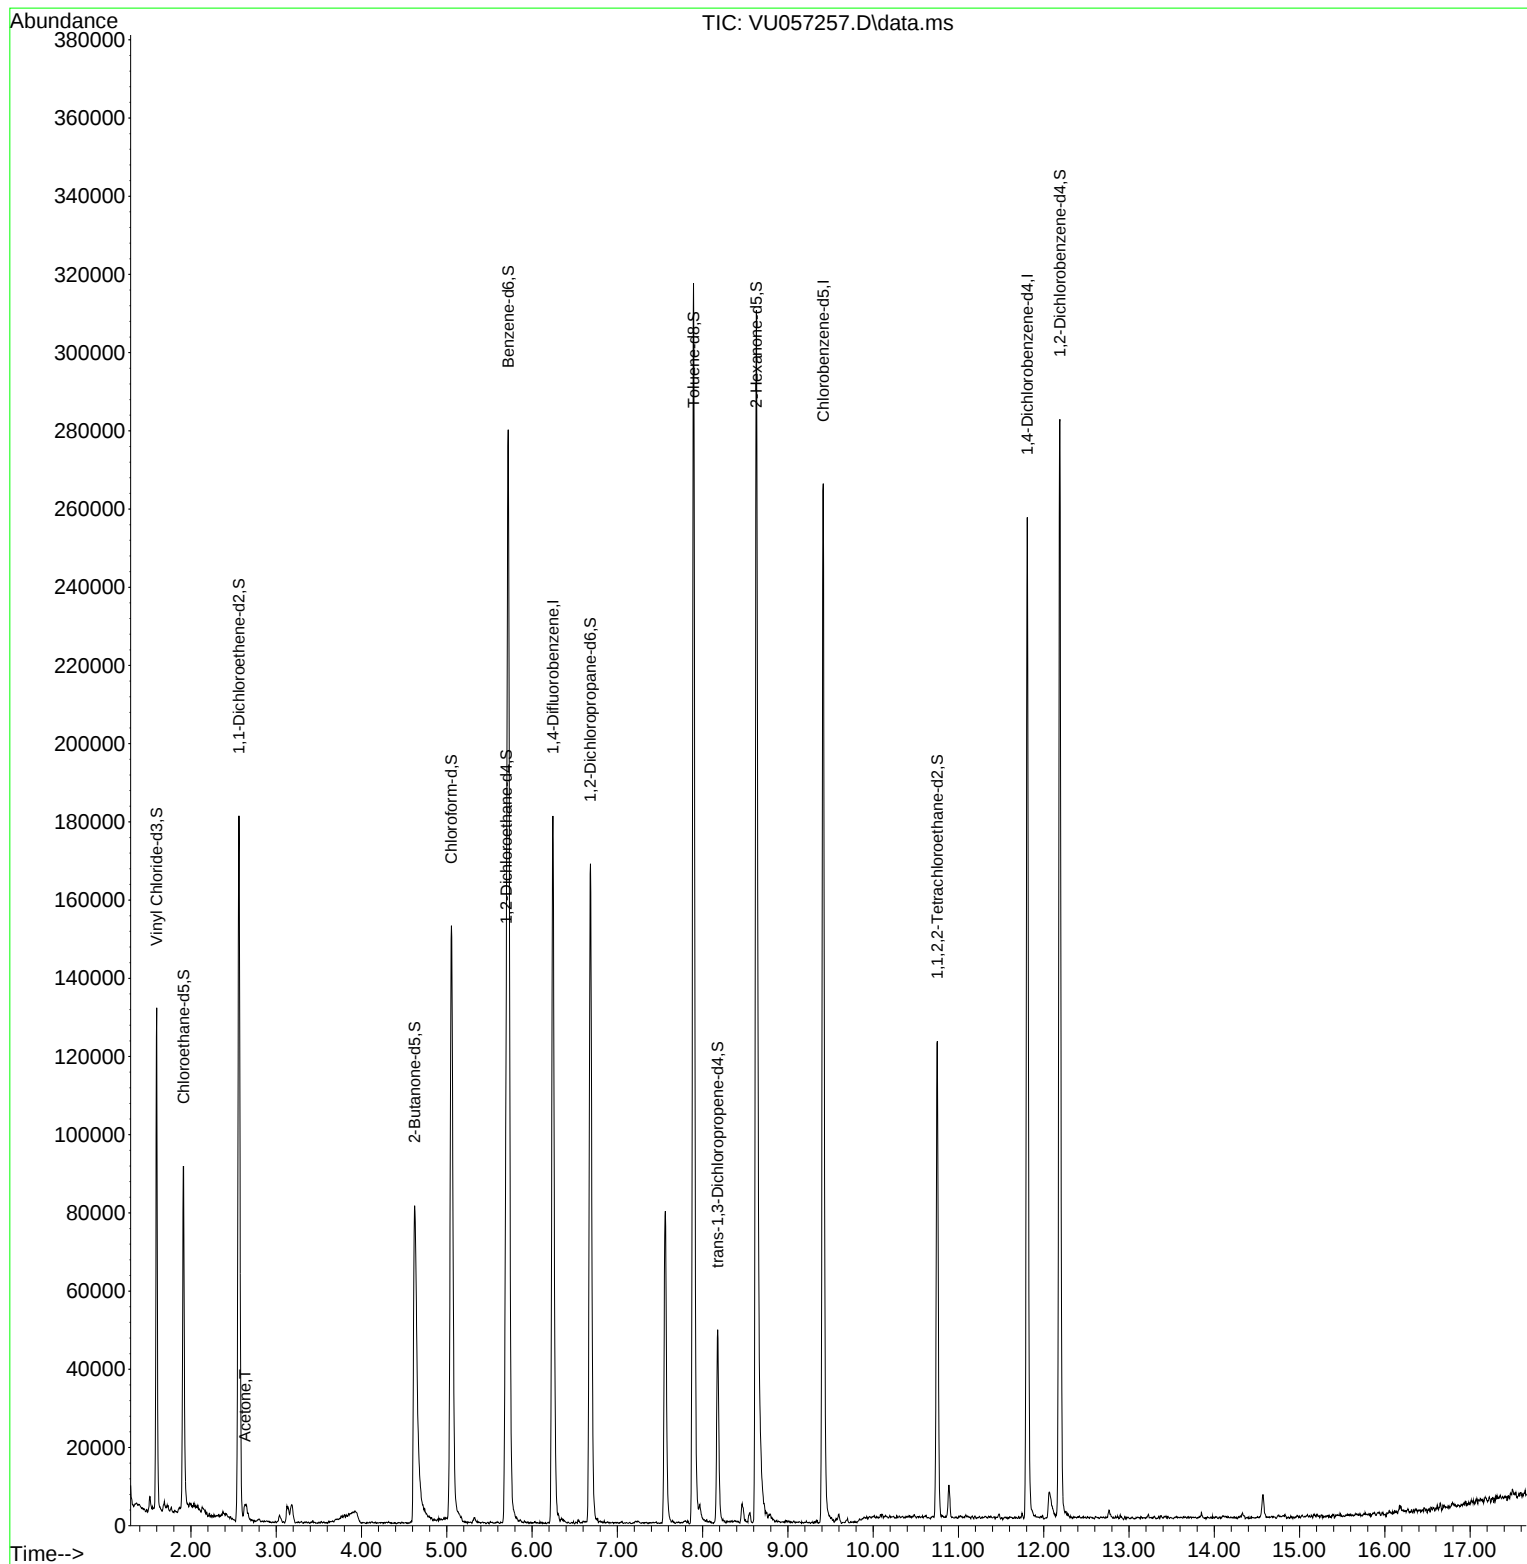

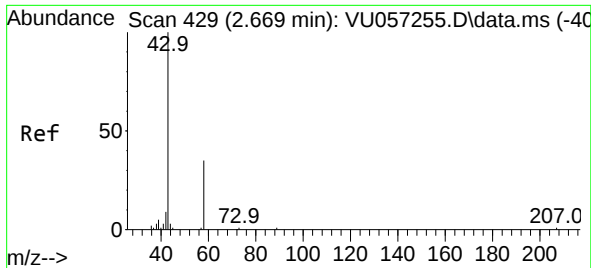

#13
 Acetone
 Concen: 6.160 ug/L m
 RT: 2.634 min Scan# 41
 Delta R.T. -0.035 min
 Lab File: VU057257.D
 Acq: 27 Dec 2023 02:07

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AG1

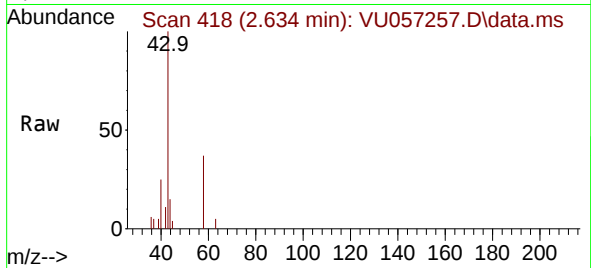

Tgt Ion: 43 Resp: 8038
 Ion Ratio Lower Upper
 43 100
 58 28.2 0.0 70.8

Manual Integrations
 APPROVED

Reviewed By :John Carlone 12/29/2023
 Supervised By :Mahesh Dadoda 12/29/2023

