

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122623\
 Data File : VU057262.D
 Acq On : 27 Dec 2023 04:09
 Operator : MD/SY
 Sample : 06002-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK9

Quant Time: Dec 27 05:48:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 27 01:05:12 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.245	114	157568	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	164345	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	73287	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.599	65	81164	5.389	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	107.800%
7) Chloroethane-d5	1.914	69	58731	4.738	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.800%
11) 1,1-Dichloroethene-d2	2.563	65	32096	4.919	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	98.400%
20) 2-Butanone-d5	4.624	46	129886	54.929	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	109.860%
24) Chloroform-d	5.055	84	133435	4.588	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.800%
26) 1,2-Dichloroethane-d4	5.695	65	65032	4.692	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.800%
32) Benzene-d6	5.721	84	254744	4.519	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.400%
36) 1,2-Dichloropropane-d6	6.685	67	80483	5.017	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.400%
41) Toluene-d8	7.894	98	206517	4.013	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	80.200%
43) trans-1,3-Dichloroprop...	8.177	79	28435	4.258	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.200%
46) 2-Hexanone-d5	8.630	63	98859	43.484	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	86.960%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	57321	5.022	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.400%
66) 1,2-Dichlorobenzene-d4	12.187	152	70674	4.482	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	89.600%
Target Compounds						
					Qvalue	
3) Chloromethane	1.518	50	5250	0.407	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122623\
Data File : VU057262.D
Acq On : 27 Dec 2023 04:09
Operator : MD/SY
Sample : 06002-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AK9

Quant Time: Dec 27 05:48:28 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Dec 27 01:05:12 2023
Response via : Initial Calibration

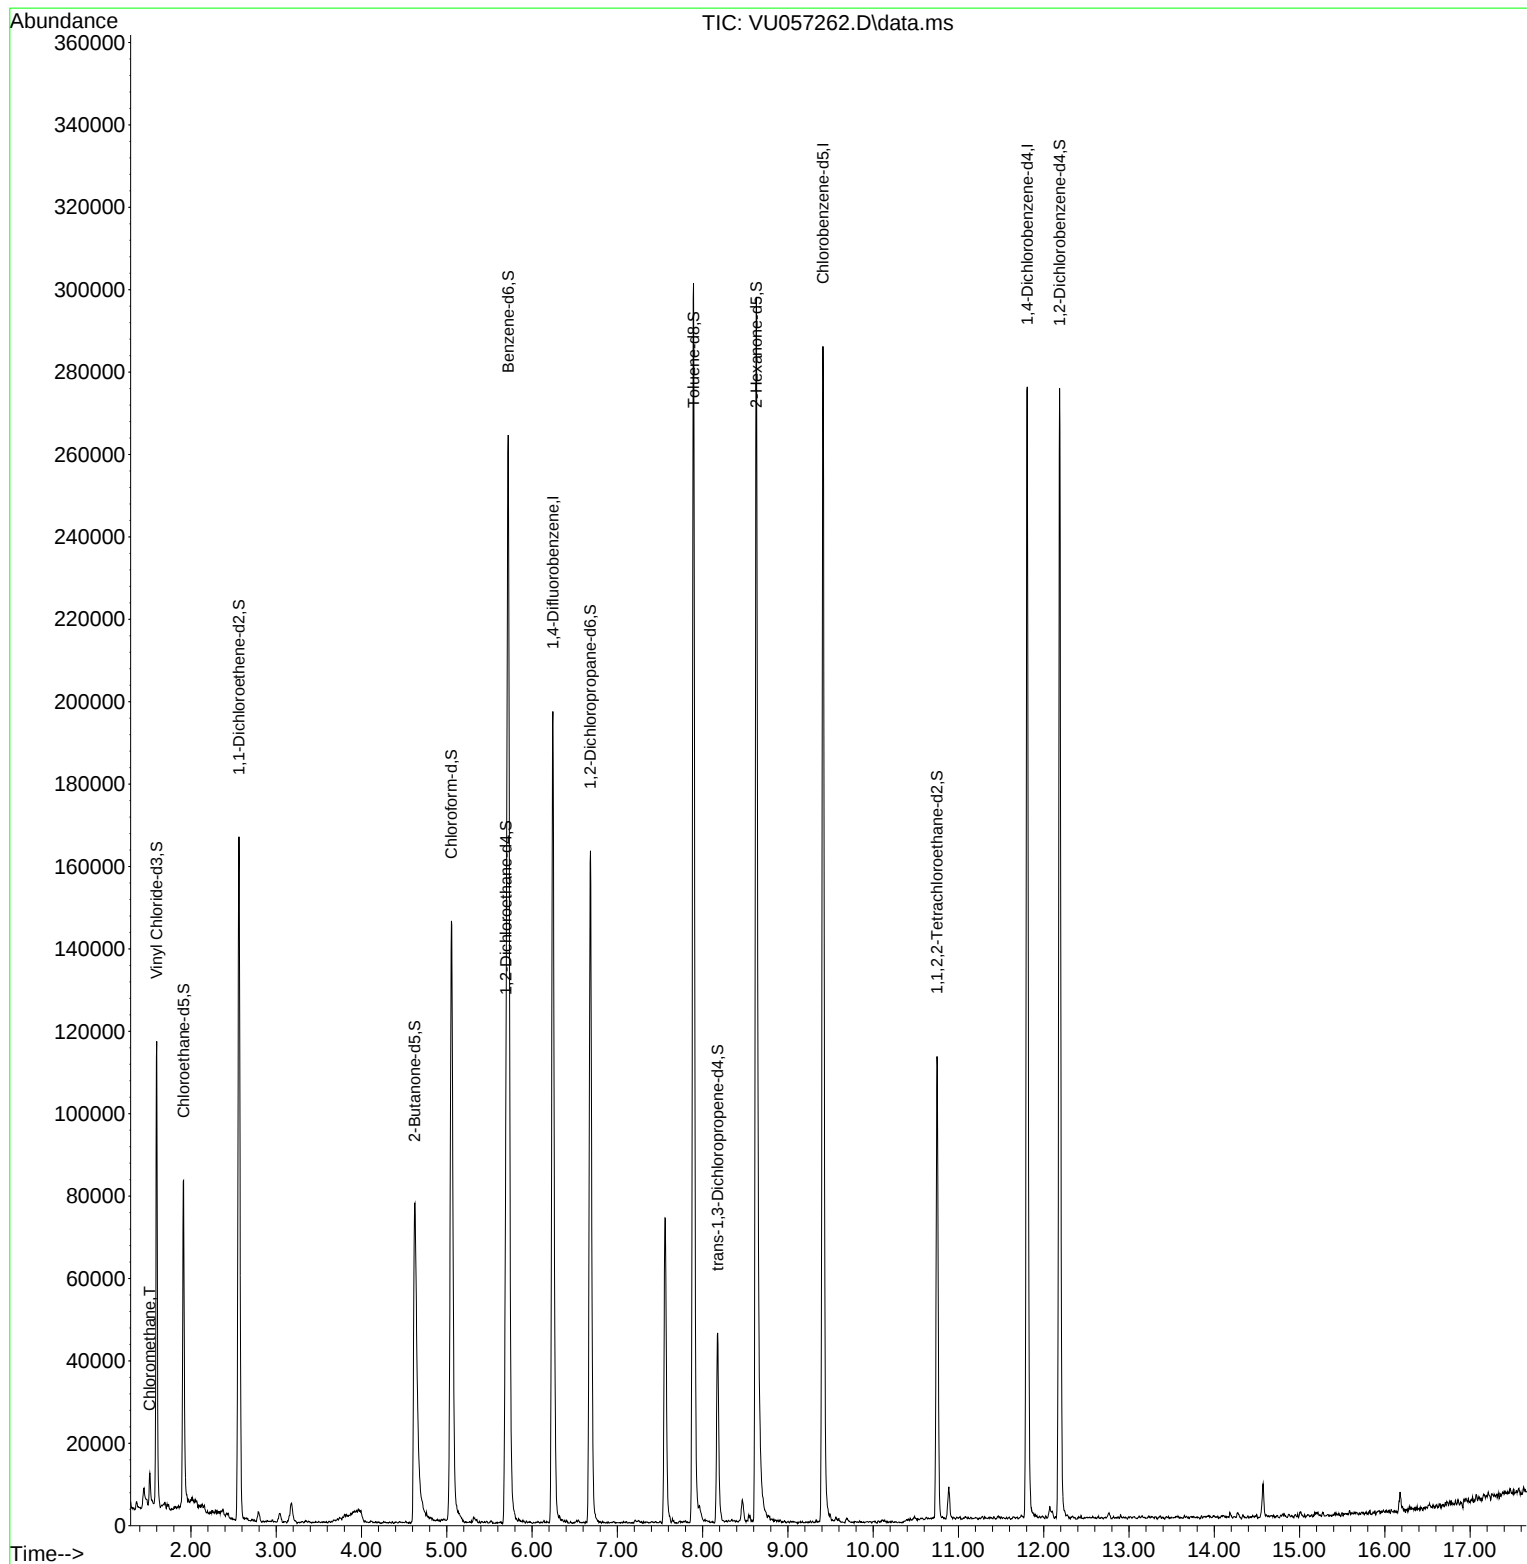

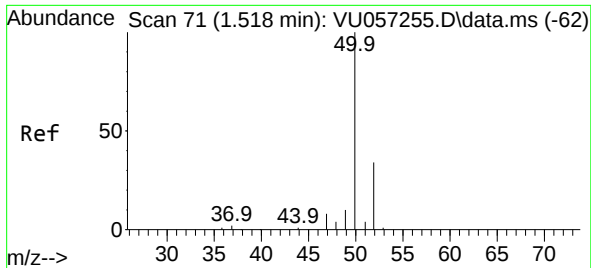

#3
 Chloromethane
 Concen: 0.407 ug/L
 RT: 1.518 min Scan# 71
 Delta R.T. -0.000 min
 Lab File: VU057262.D
 Acq: 27 Dec 2023 04:09

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AK9

Tgt Ion: 50 Resp: 5250
 Ion Ratio Lower Upper
 50 100
 52 33.0 23.7 44.1

