

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122623\
 Data File : VU057263.D
 Acq On : 27 Dec 2023 04:33
 Operator : MD/SY
 Sample : 06002-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM5

Quant Time: Dec 27 05:48:42 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Dec 27 01:05:12 2023
 Response via : Initial Calibration

Compound			R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards								
1) 1,4-Difluorobenzene			6.245	114	150541	5.000	ug/L	0.00
28) Chlorobenzene-d5			9.412	117	160289	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4			11.807	152	69407	5.000	ug/L	0.00
System Monitoring Compounds								
4) Vinyl Chloride-d3			1.596	65	86491	6.011	ug/L	0.00
Spiked Amount 5.000			Range 40 - 130		Recovery	= 120.200%		
7) Chloroethane-d5			1.911	69	65066	5.494	ug/L	0.00
Spiked Amount 5.000			Range 65 - 130		Recovery	= 109.800%		
11) 1,1-Dichloroethene-d2			2.563	65	34595	5.549	ug/L	0.00
Spiked Amount 5.000			Range 60 - 125		Recovery	= 111.000%		
20) 2-Butanone-d5			4.624	46	141355	62.570	ug/L	-0.02
Spiked Amount 50.000			Range 40 - 130		Recovery	= 125.140%		
24) Chloroform-d			5.055	84	143685	5.171	ug/L	0.00
Spiked Amount 5.000			Range 70 - 125		Recovery	= 103.400%		
26) 1,2-Dichloroethane-d4			5.695	65	71977	5.435	ug/L	0.00
Spiked Amount 5.000			Range 70 - 130		Recovery	= 108.800%		
32) Benzene-d6			5.721	84	271138	4.932	ug/L	0.00
Spiked Amount 5.000			Range 70 - 125		Recovery	= 98.600%		
36) 1,2-Dichloropropane-d6			6.685	67	83942	5.365	ug/L	0.00
Spiked Amount 5.000			Range 60 - 140		Recovery	= 107.400%		
41) Toluene-d8			7.894	98	220561	4.394	ug/L	0.00
Spiked Amount 5.000			Range 70 - 130		Recovery	= 87.800%		
43) trans-1,3-Dichloroprop...			8.177	79	30278	4.649	ug/L	0.00
Spiked Amount 5.000			Range 55 - 130		Recovery	= 93.000%		
46) 2-Hexanone-d5			8.628	63	114304	51.550	ug/L	0.00
Spiked Amount 50.000			Range 45 - 130		Recovery	= 103.100%		
56) 1,1,2,2-Tetrachloroeth...			10.750	84	61729	5.545	ug/L	0.00
Spiked Amount 5.000			Range 65 - 120		Recovery	= 110.800%		
66) 1,2-Dichlorobenzene-d4			12.187	152	76303	5.109	ug/L	0.00
Spiked Amount 5.000			Range 80 - 120		Recovery	= 102.200%		
Target Compounds								Qvalue
3) Chloromethane			1.518	50	14659	1.188	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122623\
Data File : VU057263.D
Acq On : 27 Dec 2023 04:33
Operator : MD/SY
Sample : 06002-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AM5

Quant Time: Dec 27 05:48:42 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Dec 27 01:05:12 2023
Response via : Initial Calibration

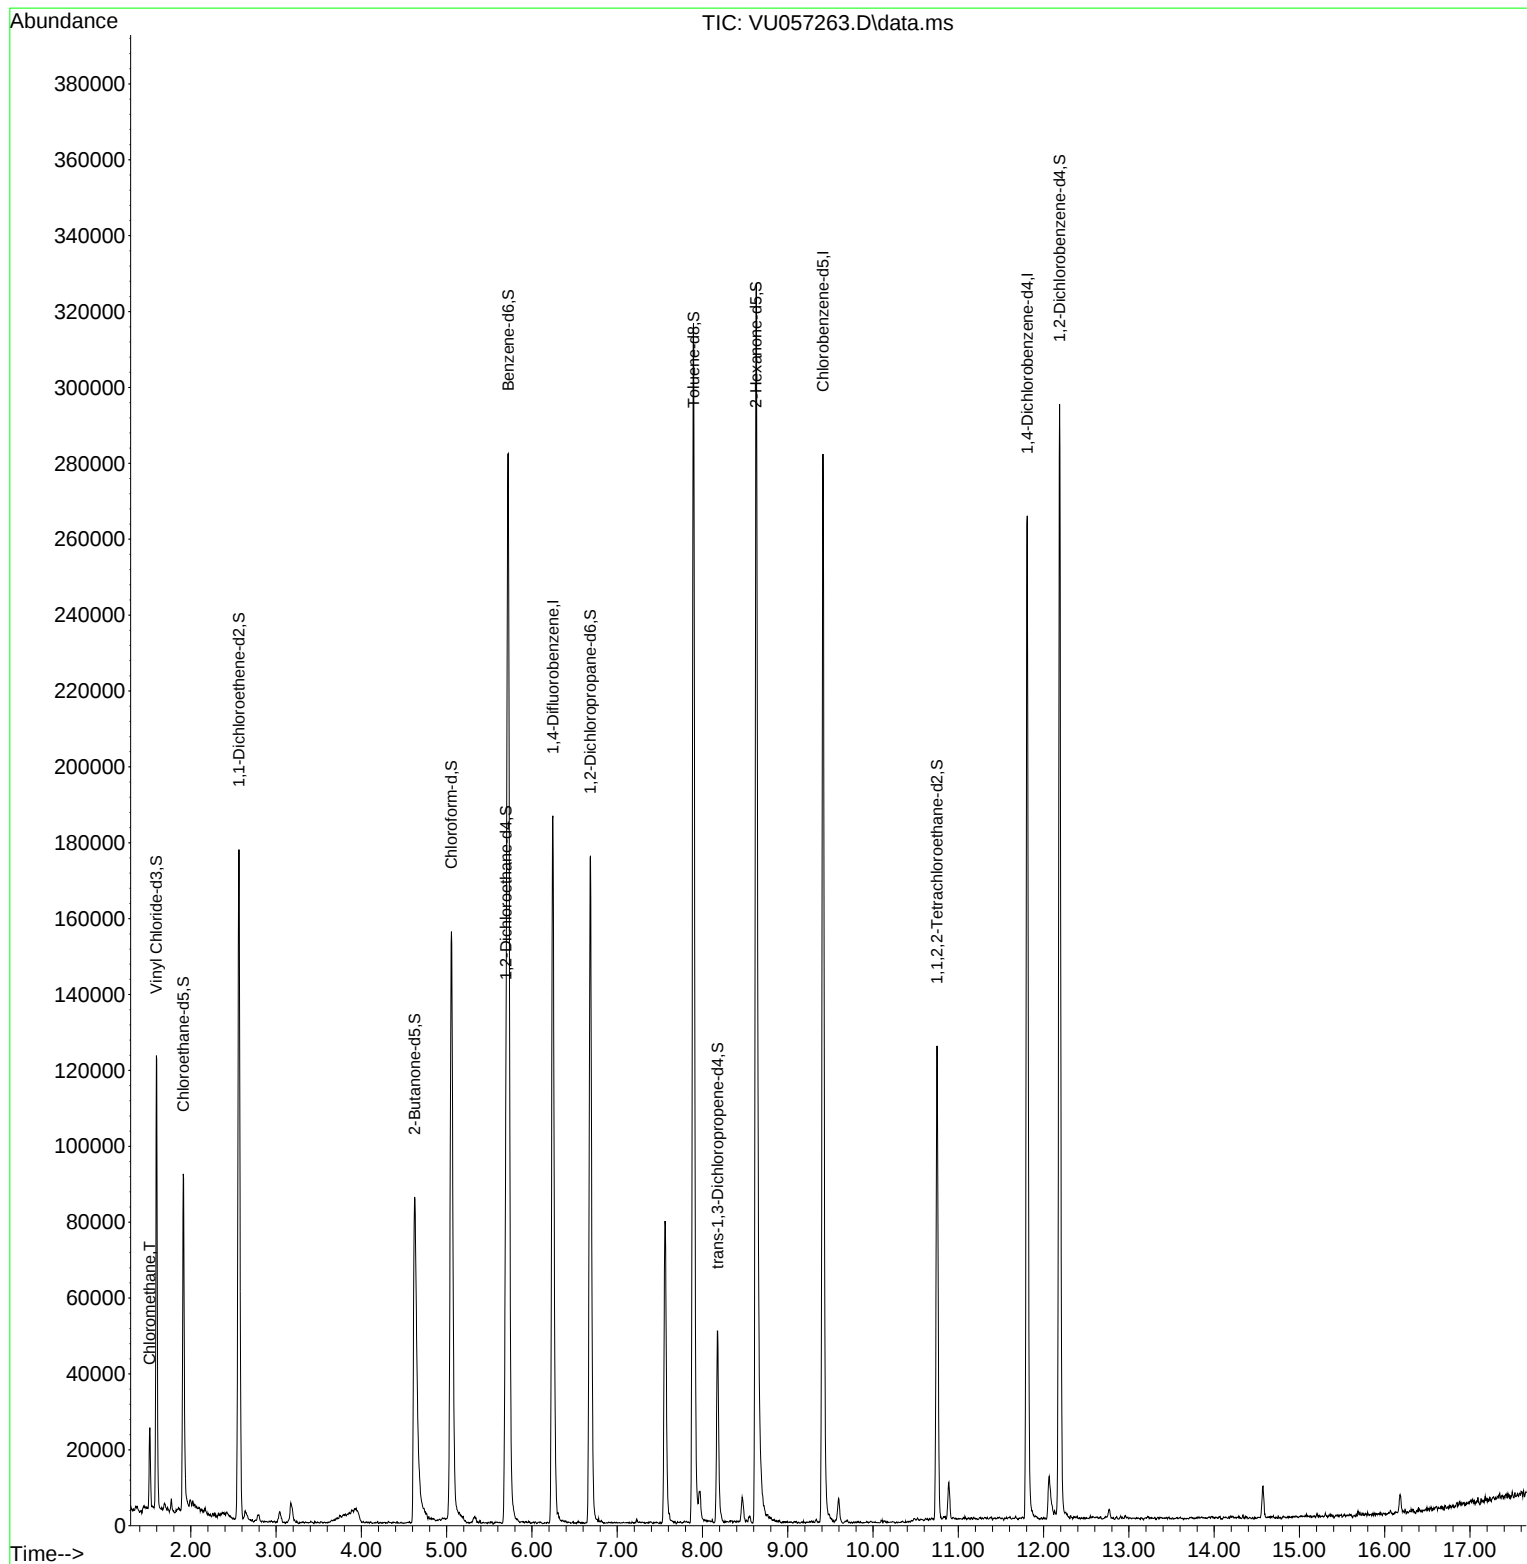

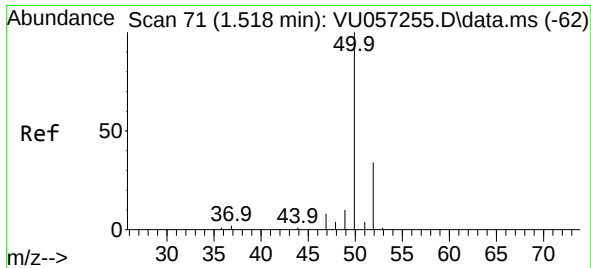

#3
 Chloromethane
 Concen: 1.188 ug/L
 RT: 1.518 min Scan# 71
 Delta R.T. 0.000 min
 Lab File: VU057263.D
 Acq: 27 Dec 2023 04:33

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AM5

Tgt Ion: 50 Resp: 14659
 Ion Ratio Lower Upper
 50 100
 52 30.8 23.7 44.1

