

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122623\
 Data File : VU057241.D
 Acq On : 26 Dec 2023 17:58
 Operator : MD/SY
 Sample : 05927-15
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU057241.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	88	95	105	rVB	125524	137752	20.30%	2.579%
2	1.911	184	193	212	rVB	85026	117873	17.37%	2.207%
3	2.563	383	396	412	rBV	170215	278231	41.00%	5.210%
4	3.177	576	587	597	rBV	4233	8390	1.24%	0.157%
5	4.621	1016	1036	1072	rBV	83522	221525	32.64%	4.148%
6	5.055	1153	1171	1194	rBV	138110	311835	45.95%	5.839%
7	5.718	1357	1377	1402	rBV3	263489	678644	100.00%	12.707%
8	6.245	1527	1541	1561	rBV	185809	359596	52.99%	6.733%
9	6.541	1620	1633	1644	rVB9	5381	9975	1.47%	0.187%
10	6.685	1665	1678	1699	rBV2	163431	314341	46.32%	5.886%
11	7.560	1936	1950	1970	rBV2	76424	137997	20.33%	2.584%
12	7.894	2039	2054	2076	rBV	299508	536808	79.10%	10.051%
13	8.177	2130	2142	2158	rBV	46816	83450	12.30%	1.563%
14	8.467	2222	2232	2247	rVB3	10347	18899	2.78%	0.354%
15	8.627	2269	2282	2320	rBV	280447	565739	83.36%	10.593%
16	9.412	2514	2526	2550	rBV	270183	466773	68.78%	8.740%
17	10.749	2931	2942	2955	rBV2	106165	177642	26.18%	3.326%
18	10.888	2970	2985	2999	rBV2	17120	27464	4.05%	0.514%
19	11.807	3259	3271	3290	rBV	254562	425417	62.69%	7.966%
20	12.187	3373	3389	3415	rBV2	258619	440135	64.86%	8.241%
21	14.569	4119	4130	4143	rBV	13668	22251	3.28%	0.417%




Sum of corrected areas: 5340737

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122623\
Data File : VU057241.D
Acq On : 26 Dec 2023 17:58
Operator : MD/SY
Sample : 05927-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

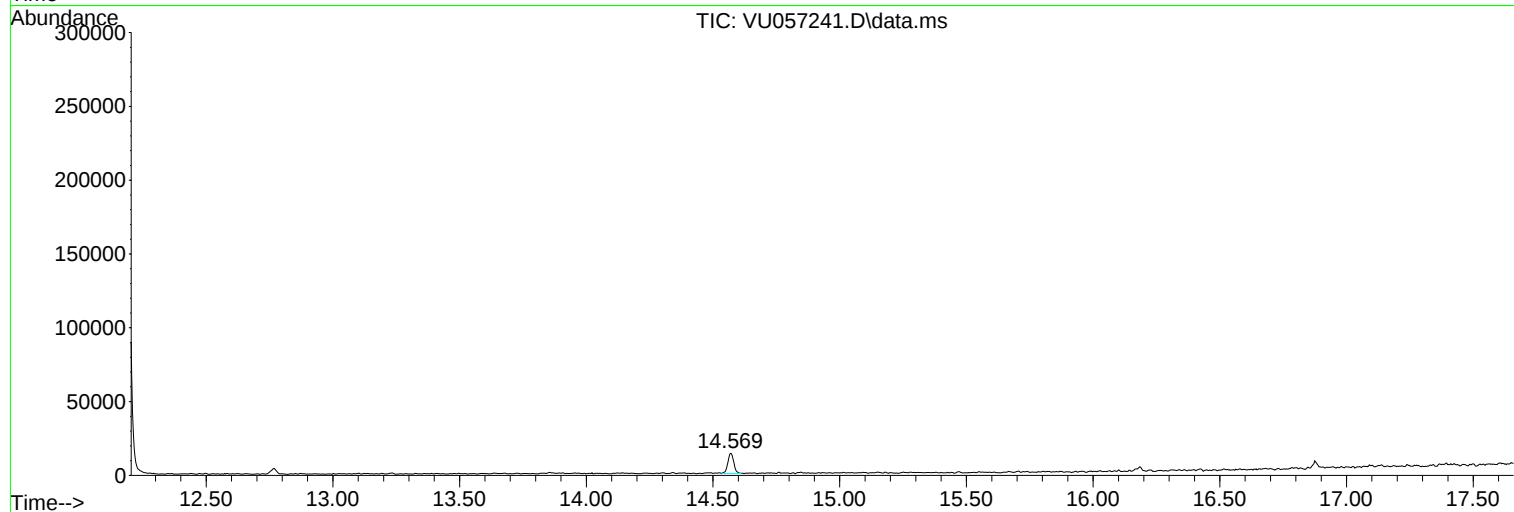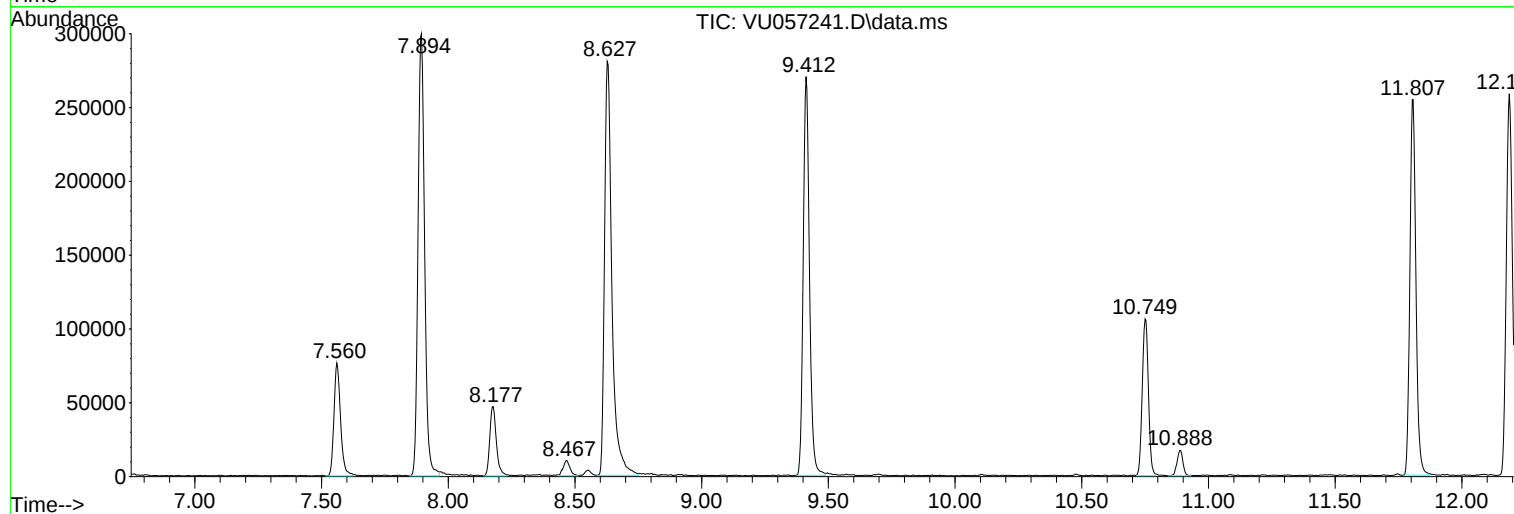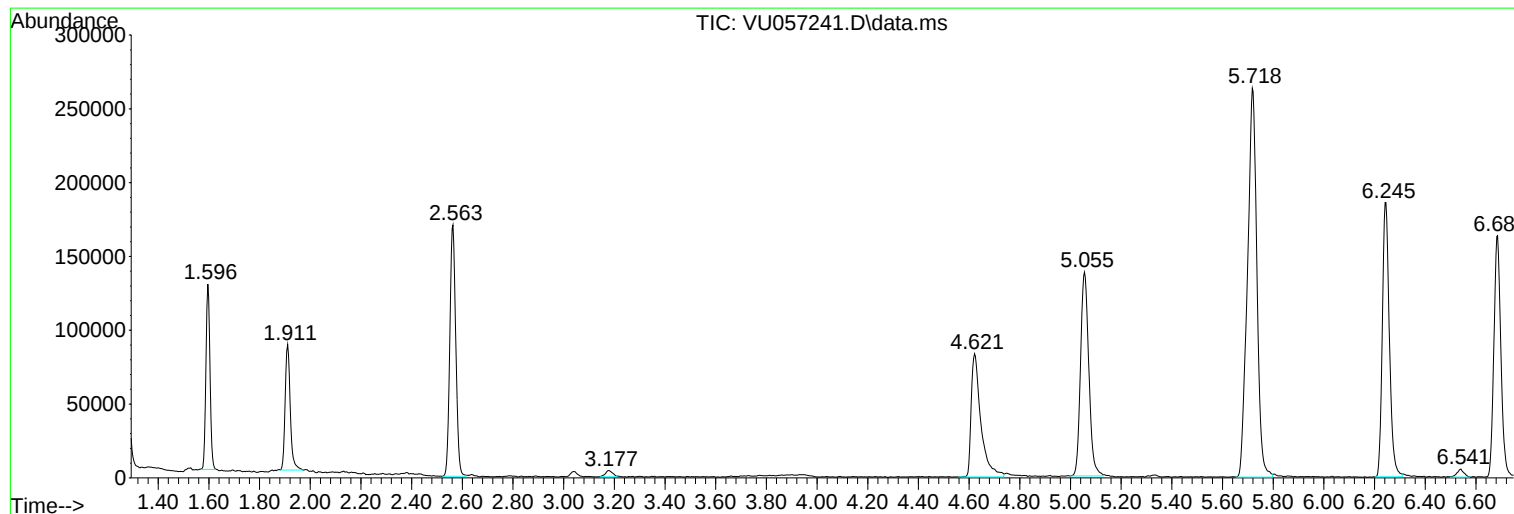

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122623\
Data File : VU057241.D
Acq On : 26 Dec 2023 17:58
Operator : MD/SY
Sample : 05927-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122623\
Data File : VU057241.D
Acq On : 26 Dec 2023 17:58
Operator : MD/SY
Sample : 05927-15
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc