

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122623\
 Data File : VU057246.D
 Acq On : 26 Dec 2023 19:59
 Operator : MD/SY
 Sample : 05976-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BH7W2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU057246.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	107	rVB	118321	131901	20.19%	2.084%
2	1.727	128	136	147	rVB	36832	44454	6.81%	0.702%
3	1.911	184	193	205	rBV	83515	115778	17.73%	1.829%
4	2.560	383	395	411	rBV	161000	267468	40.95%	4.225%
5	2.644	414	421	440	rVB6	3324	7883	1.21%	0.125%
6	3.178	566	587	606	rBV	115607	265822	40.70%	4.199%
7	3.866	789	801	805	rBV3	5378	9529	1.46%	0.151%
8	4.628	1019	1038	1076	rBV5	154251	638359	97.73%	10.084%
9	5.055	1156	1171	1196	rBV	132696	304959	46.69%	4.817%
10	5.313	1235	1251	1271	rVB3	37467	91109	13.95%	1.439%
11	5.718	1356	1377	1400	rBV3	255012	653170	100.00%	10.318%
12	6.242	1528	1540	1562	rBV	185396	360640	55.21%	5.697%
13	6.538	1618	1632	1659	rBV	167154	318459	48.76%	5.030%
14	6.682	1665	1677	1695	rBV2	152768	300046	45.94%	4.740%
15	7.560	1940	1950	1970	rBV	73032	129830	19.88%	2.051%
16	7.891	2040	2053	2069	rBV	287349	508661	77.88%	8.035%
17	8.174	2131	2141	2156	rBV2	44763	78256	11.98%	1.236%
18	8.467	2219	2232	2243	rBV4	10921	19351	2.96%	0.306%
19	8.628	2270	2282	2313	rBV2	275608	546937	83.74%	8.640%
20	9.412	2514	2526	2552	rBV	266993	466840	71.47%	7.374%
21	10.750	2930	2942	2957	rBV	106575	170909	26.17%	2.700%
22	10.888	2975	2985	2997	rVB3	16415	26775	4.10%	0.423%
23	11.807	3259	3271	3296	rBV	254067	413121	63.25%	6.526%
24	12.187	3376	3389	3409	rBV	253203	423608	64.85%	6.691%
25	14.569	4121	4130	4141	rVB	16285	26238	4.02%	0.414%
26	16.180	4620	4631	4638	rBV3	6743	10476	1.60%	0.165%




Sum of corrected areas: 6330579

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122623\
Data File : VU057246.D
Acq On : 26 Dec 2023 19:59
Operator : MD/SY
Sample : 05976-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH7W2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

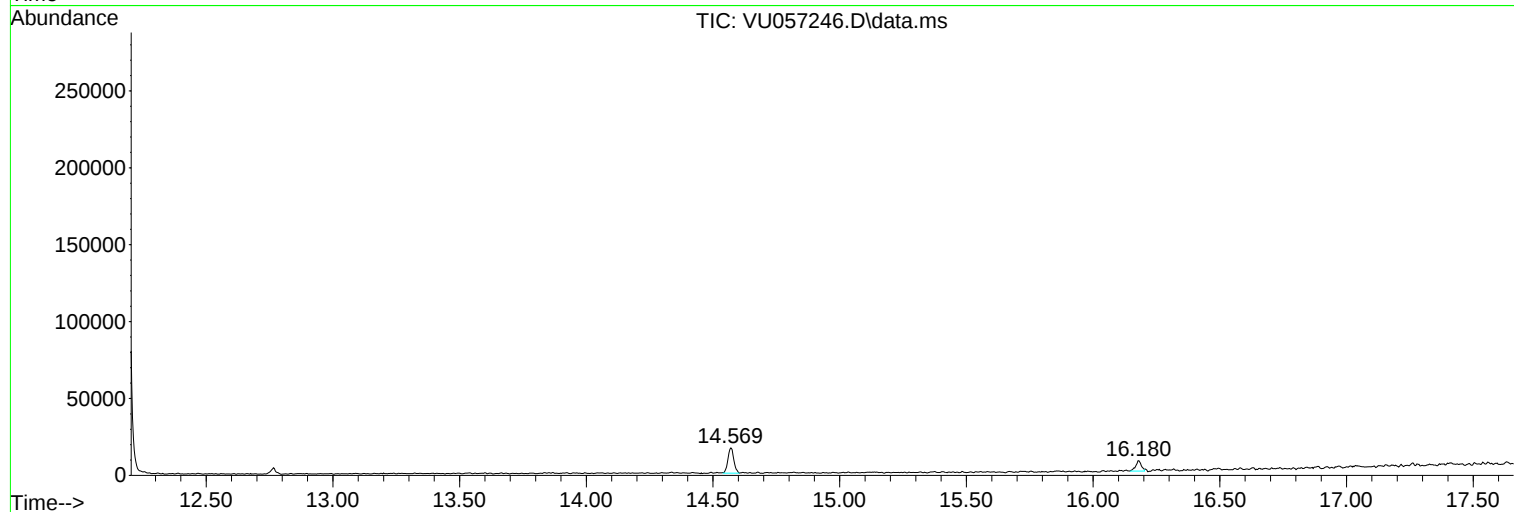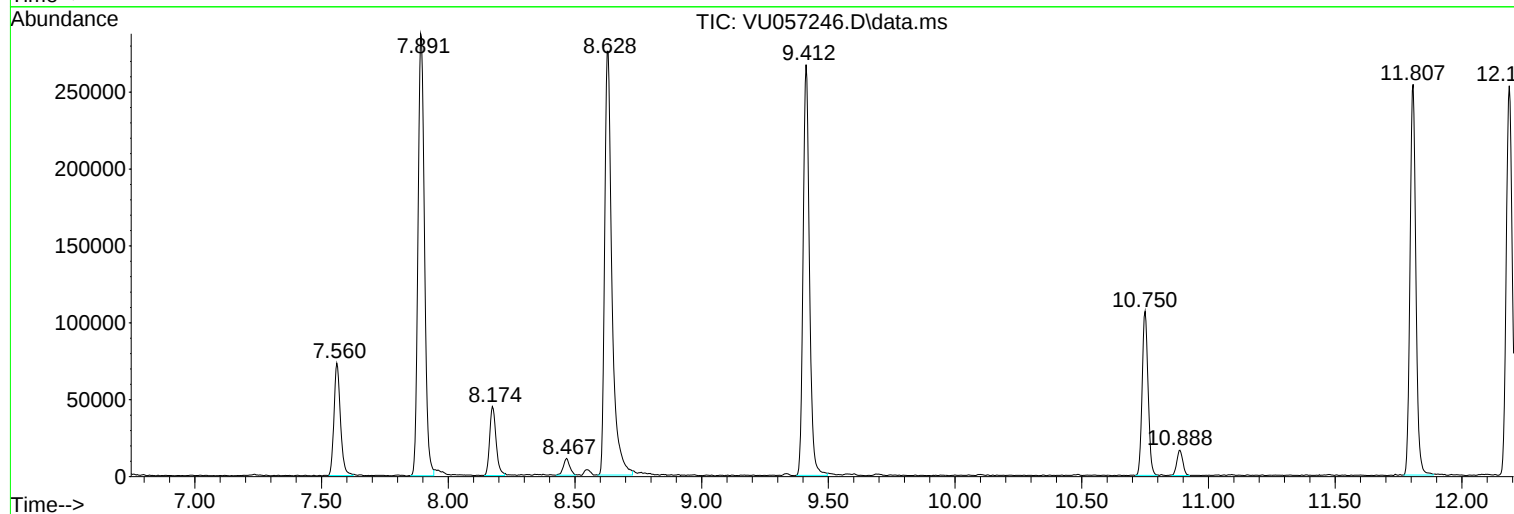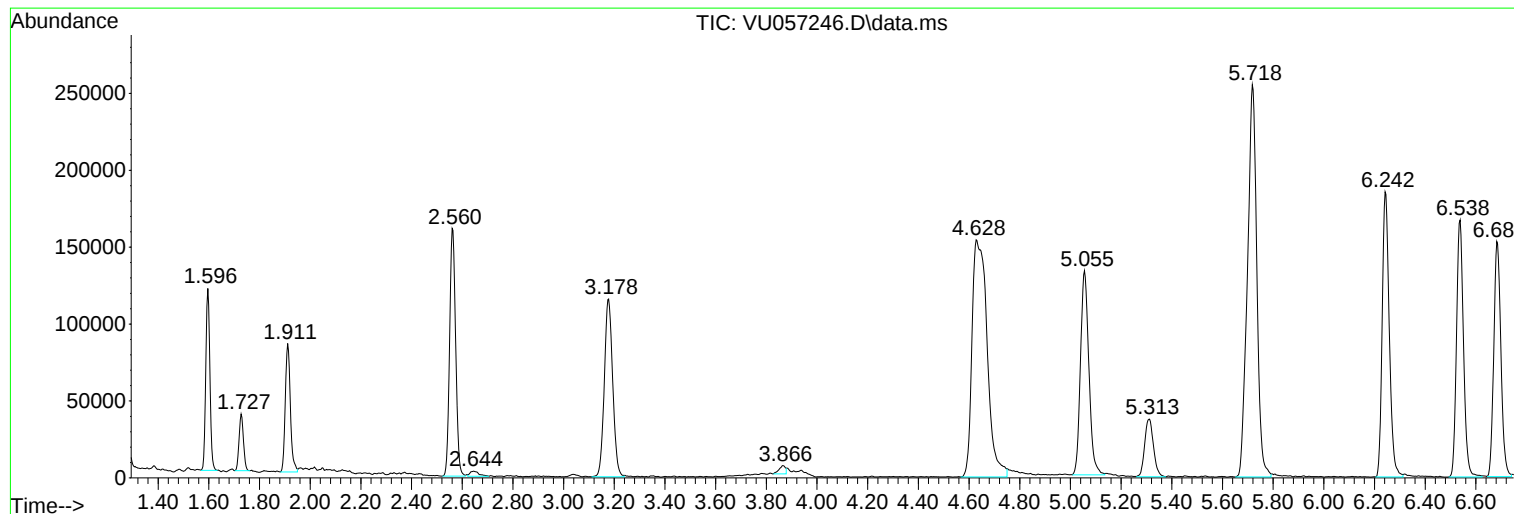

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122623\
Data File : VU057246.D
Acq On : 26 Dec 2023 19:59
Operator : MD/SY
Sample : 05976-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH7W2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122623\
Data File : VU057246.D
Acq On : 26 Dec 2023 19:59
Operator : MD/SY
Sample : 05976-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BH7W2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------