


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122623\
Data File : VU057234.D
Acq On : 26 Dec 2023 13:23
Operator : MD/SY
Sample : BFB101
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB101

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR122123WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Dec 27 01:05:12 2023

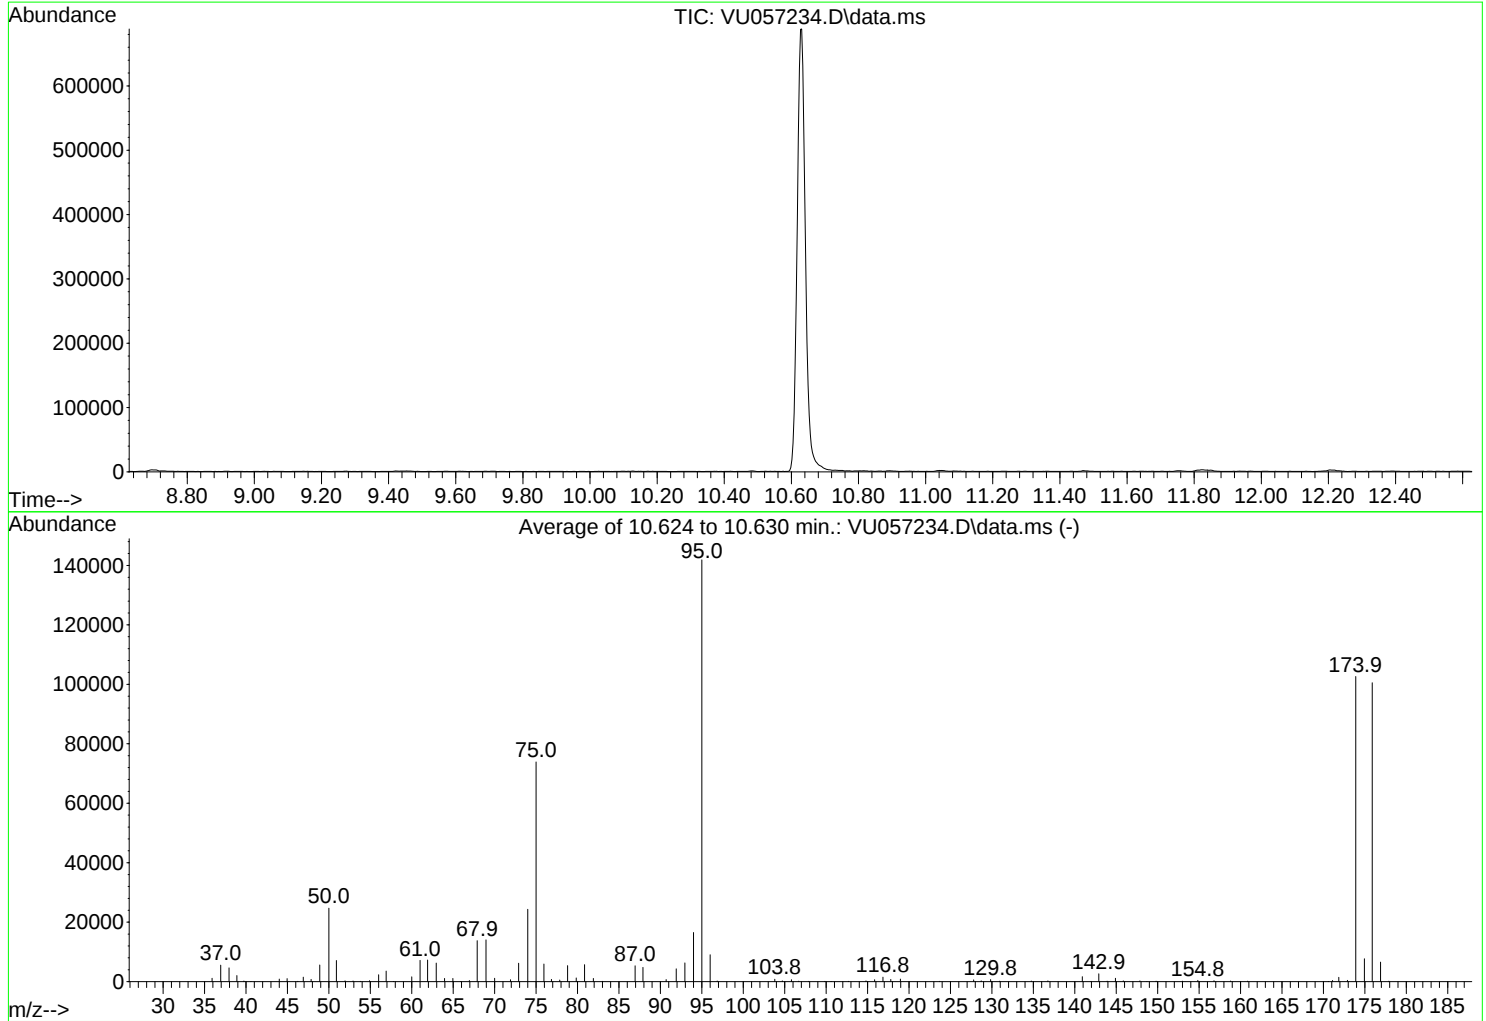

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	24696	PASS
75	95	30	80	52.1	73869	PASS
95	95	100	100	100.0	141867	PASS
96	95	5	9	6.4	9025	PASS
173	174	0.00	2	0.4	449	PASS
174	95	50	120	72.3	102616	PASS
175	174	5	9	7.5	7699	PASS
176	174	95	101	98.0	100557	PASS
177	176	5	9	6.5	6548	PASS

m/z	Abundance
39.70	365.0
44.10	301.0

Instrument :
MSVOA_U
ClientSampleId :
BFB101

m/z	Abundance
35.90	1032.0
36.90	5322.0
37.90	4203.0
38.90	2058.0
39.80	557.0
40.60	125.0
44.00	1231.0
45.00	977.0
46.20	172.0
46.90	1384.0
47.90	747.0
48.90	5228.0
50.00	23672.0
50.90	6818.0
51.90	255.0
52.90	162.0
53.80	101.0
54.80	302.0
56.00	2045.0
56.90	3338.0
60.00	1364.0
61.00	6540.0
61.90	6930.0
62.90	6033.0
63.90	834.0
64.90	938.0
66.90	317.0
67.90	13242.0
69.00	13141.0
70.00	1039.0
71.90	615.0
72.90	5829.0
74.00	23560.0
75.00	70696.0
75.90	5528.0
76.80	775.0
77.90	468.0
78.80	4971.0
79.90	1044.0
80.90	5309.0
81.90	1035.0
87.00	5326.0
87.90	4446.0
90.70	660.0
91.90	4007.0
92.90	6110.0
94.00	15818.0
95.00	133760.0
96.00	8964.0
96.80	168.0
103.80	817.0
104.70	302.0
105.80	551.0
106.70	127.0
107.90	125.0
109.80	142.0
110.60	130.0
112.70	168.0
114.80	212.0
115.90	646.0
116.80	1483.0
117.80	814.0
118.90	892.0
123.70	133.0
127.80	539.0
128.70	166.0
129.90	582.0
131.00	198.0
134.80	223.0
136.80	276.0
140.90	1621.0
142.00	152.0
142.90	2412.0
144.00	126.0
144.90	1113.0
145.90	231.0
147.80	229.0
149.80	154.0
153.00	118.0
154.90	405.0
156.80	287.0
158.70	160.0
160.90	198.0
171.00	344.0
171.90	1481.0
172.90	1347.0
173.90	94216.0
174.90	7209.0
175.90	91968.0
176.90	6082.0
177.90	185.0

Instrument :
MSVOA_U
ClientSampleId :
BFB101

m/z	Abundance
35.90	1172.0
36.90	5632.0
38.00	4717.0
38.90	2188.0
39.80	590.0
44.00	1232.0
44.90	1032.0
46.30	233.0
46.90	1576.0
47.80	758.0
48.90	5858.0
50.00	25576.0
50.90	7444.0
52.00	272.0
52.90	218.0
53.80	109.0
54.90	312.0
56.00	2461.0
56.90	3663.0
57.80	118.0
60.00	1696.0
61.00	7437.0
61.90	7518.0
63.00	6390.0
64.00	1088.0
65.00	1121.0
67.00	376.0
67.90	14327.0
69.00	14376.0
70.00	1184.0
71.90	695.0
72.90	6336.0
74.00	24960.0
75.00	76144.0
75.90	6071.0
76.90	752.0
77.90	539.0
78.80	5563.0
79.90	1298.0
80.80	5947.0
81.90	1120.0
83.00	126.0
87.00	5393.0
87.90	4852.0
90.70	740.0
91.90	4448.0
92.90	6450.0
94.00	16712.0
95.00	145984.0
96.00	9324.0
96.90	206.0
103.80	835.0
104.70	282.0
105.80	670.0
106.70	138.0
107.90	154.0
109.80	125.0
110.60	129.0
112.70	131.0
114.80	274.0
115.90	693.0
116.80	1535.0
117.80	783.0
119.00	858.0
123.70	164.0
127.80	596.0
128.70	285.0
129.80	704.0
131.00	184.0
134.80	235.0
136.70	297.0
140.90	1723.0
142.00	134.0
142.90	2671.0
143.90	152.0
144.90	1189.0
145.80	281.0
147.80	275.0
149.80	160.0
153.00	208.0
154.90	463.0
156.80	327.0
158.80	196.0
160.90	186.0
171.10	390.0
171.90	1470.0
173.90	105800.0
174.90	7832.0
175.90	103992.0
176.90	6727.0
177.90	177.0

Instrument :
MSVOA_U
ClientSampleId :
BFB101

m/z	Abundance
35.90	1156.0
37.00	5648.0
38.00	4999.0
38.90	1981.0
39.90	643.0
44.00	1107.0
44.90	994.0
46.90	1590.0
47.80	786.0
48.90	5779.0
50.00	24840.0
50.90	7136.0
52.00	268.0
52.90	220.0
53.80	102.0
55.00	307.0
56.00	2468.0
56.90	3628.0
57.80	103.0
60.00	1853.0
61.00	7481.0
61.90	7318.0
62.90	6355.0
64.00	1255.0
65.00	1115.0
65.90	104.0
67.00	402.0
67.90	13797.0
68.90	14585.0
70.00	1167.0
71.90	687.0
72.90	6457.0
74.00	24528.0
75.00	74768.0
76.00	6132.0
76.90	727.0
77.80	650.0
78.80	5604.0
79.80	1470.0
80.80	5798.0
81.90	1135.0
83.00	149.0
86.90	5288.0
87.90	5130.0
90.70	669.0
91.90	4522.0
93.00	6298.0
94.00	17112.0
95.00	145856.0
96.00	8787.0
96.90	240.0
103.80	704.0
104.70	234.0
105.80	720.0
106.70	182.0
107.90	112.0
109.90	119.0
114.80	279.0
115.80	629.0
116.90	1461.0
117.80	653.0
118.90	778.0
123.70	104.0
127.80	611.0
128.70	331.0
129.90	784.0
130.90	167.0
134.70	245.0
136.80	292.0
140.90	1722.0
141.80	115.0
142.90	2820.0
143.80	188.0
144.90	1099.0
145.80	280.0
147.90	325.0
148.70	120.0
149.80	136.0
153.00	201.0
154.80	419.0
156.80	308.0
158.90	225.0
160.80	183.0
170.60	248.0
171.20	395.0
171.80	1351.0
173.90	107832.0
175.00	8056.0
175.90	105712.0
176.90	6834.0
177.90	149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB101