
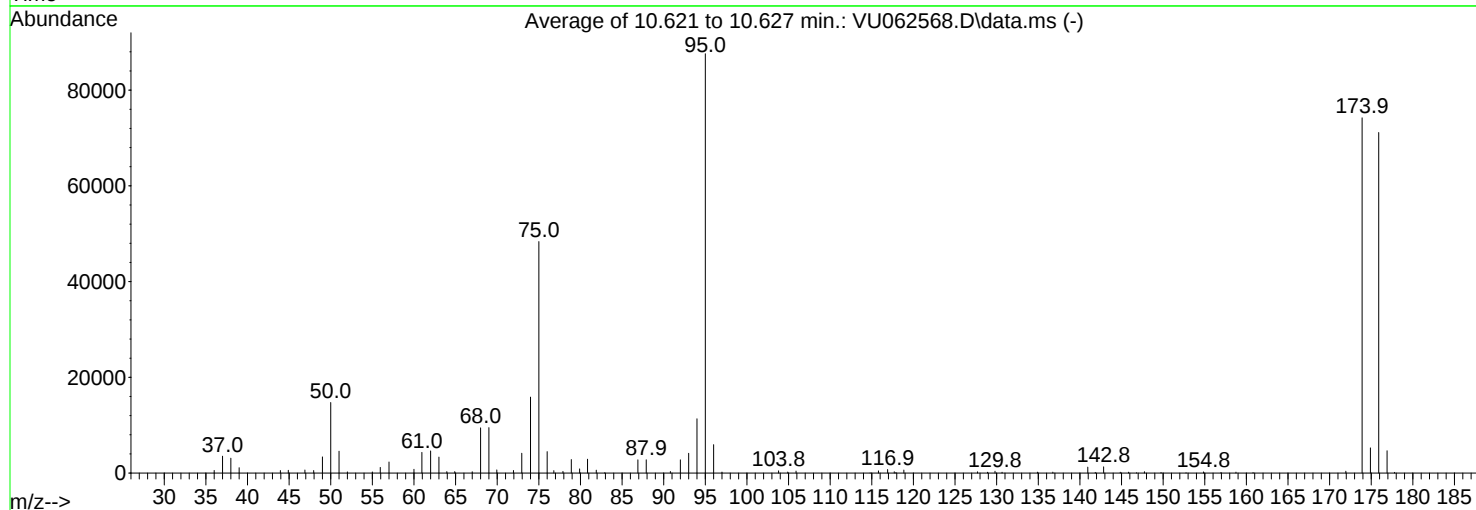


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU122624\
Data File : VU062568.D
Acq On : 26 Dec 2024 09:58
Operator : MD/SY
Sample : BFB053
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB053

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR120924WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Dec 27 01:06:59 2024

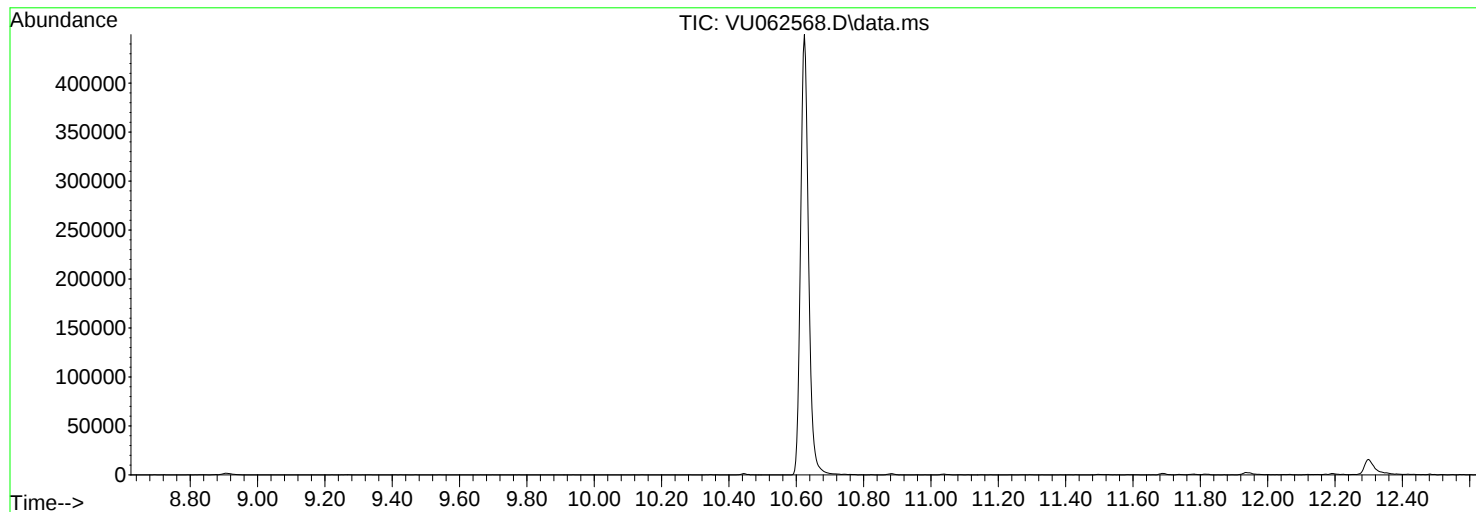

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2889

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	14741	PASS
75	95	30	80	55.2	48363	PASS
95	95	100	100	100.0	87600	PASS
96	95	5	9	6.8	5941	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.7	74208	PASS
175	174	5	9	7.1	5263	PASS
176	174	95	101	95.9	71147	PASS
177	176	5	9	6.6	4669	PASS

Scan 2889 (10.579 min): VU062568.D
\\data.ms BFB053

m/z Abundance

Instrument :
MSVOA_U
ClientSampleId :
BFB053

m/z	Abundance
36.10	500.0
37.00	3640.0
38.00	3073.0
39.00	1158.0
43.90	584.0
44.90	582.0
46.90	626.0
48.00	474.0
49.00	3447.0
50.00	14682.0
51.00	4497.0
52.00	240.0
55.00	260.0
56.00	1142.0
57.00	2383.0
60.00	802.0
61.00	4452.0
62.00	4838.0
63.00	3286.0
63.90	387.0
64.90	327.0
67.00	325.0
68.00	9429.0
69.00	9611.0
70.00	659.0
71.00	538.0
73.00	4066.0
74.00	15859.0
75.00	49144.0
76.00	4551.0
76.80	522.0
77.90	310.0
78.90	2832.0
79.90	830.0
80.80	2906.0
81.90	570.0
82.90	102.0
86.90	2841.0
87.90	2923.0
90.80	317.0
92.00	2681.0
93.00	3906.0
94.00	11078.0
95.00	86856.0
96.00	6095.0
97.00	216.0
103.80	480.0
104.90	222.0
105.90	383.0
115.80	425.0
116.90	756.0
117.70	438.0
118.90	508.0
127.70	269.0
129.00	154.0
129.80	371.0
130.60	174.0
134.90	183.0
136.70	182.0
141.00	1217.0
141.90	131.0
142.90	1234.0
144.80	178.0
145.80	143.0
146.80	109.0
147.80	318.0
149.70	128.0
154.80	270.0
157.00	142.0
158.70	140.0
160.90	122.0
171.90	409.0
173.90	72024.0
174.90	5225.0
175.90	69200.0
176.90	4613.0
177.80	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB053

m/z	Abundance
36.00	541.0
37.00	3630.0
38.00	3183.0
39.00	1166.0
43.90	533.0
44.90	612.0
46.90	678.0
47.90	558.0
49.00	3454.0
50.00	15163.0
51.00	4788.0
52.00	263.0
55.00	252.0
56.00	1182.0
57.00	2396.0
60.00	826.0
61.00	4404.0
62.00	4844.0
63.00	3481.0
64.00	314.0
64.90	343.0
67.00	282.0
68.00	9773.0
69.00	9766.0
70.00	671.0
72.00	559.0
72.90	4267.0
74.00	16347.0
75.00	49928.0
76.00	4682.0
76.80	539.0
77.90	384.0
78.90	2916.0
79.90	912.0
80.80	2995.0
81.90	643.0
82.90	100.0
86.90	2878.0
87.90	2840.0
90.80	342.0
92.00	2886.0
93.00	4331.0
94.00	11635.0
95.00	90488.0
96.00	6075.0
97.00	229.0
103.80	500.0
104.90	227.0
105.90	454.0
114.80	105.0
115.80	465.0
116.90	780.0
117.70	410.0
118.80	654.0
127.70	277.0
128.90	177.0
129.80	401.0
130.60	196.0
134.90	215.0
136.70	215.0
140.90	1282.0
141.80	126.0
142.90	1329.0
144.90	170.0
145.90	206.0
146.80	107.0
147.80	296.0
149.70	139.0
152.70	126.0
154.90	272.0
157.00	125.0
158.70	219.0
160.80	101.0
172.00	428.0
173.90	76432.0
174.90	5443.0
175.90	73624.0
176.90	4758.0
177.80	161.0

Instrument :
MSVOA_U
ClientSampleId :
BFB053

m/z	Abundance
35.90	609.0
37.00	3330.0
38.00	3069.0
39.00	1040.0
44.00	471.0
44.90	565.0
46.90	626.0
47.90	552.0
49.00	3237.0
50.00	14377.0
51.00	4434.0
52.00	270.0
55.00	214.0
55.90	1215.0
57.00	2159.0
60.00	751.0
60.90	4118.0
62.00	4179.0
63.00	3265.0
63.90	243.0
64.90	283.0
67.00	245.0
68.00	9129.0
69.00	9098.0
69.90	671.0
72.00	528.0
72.90	4091.0
74.00	15416.0
75.00	46016.0
76.00	4226.0
76.80	479.0
77.90	359.0
78.90	2751.0
79.90	879.0
80.90	2787.0
81.90	637.0
86.90	2579.0
87.90	2565.0
90.80	353.0
92.00	2730.0
93.00	4169.0
94.00	11311.0
95.00	85456.0
96.00	5654.0
97.00	201.0
103.80	446.0
104.90	205.0
105.90	436.0
115.80	504.0
116.90	696.0
117.90	384.0
118.80	725.0
127.70	284.0
128.80	214.0
129.80	413.0
130.70	172.0
134.90	216.0
136.80	203.0
140.90	1234.0
141.80	165.0
142.80	1349.0
144.90	194.0
145.90	232.0
147.70	252.0
149.80	130.0
152.80	100.0
154.80	227.0
156.90	118.0
158.80	247.0
160.70	116.0
171.90	357.0
173.90	74168.0
174.90	5120.0
175.90	70616.0
176.90	4635.0
177.80	149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB053