


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU122718\
Data File : VU028953.D
Acq On : 27 Dec 2018 08:25
Operator : MD/SY
Sample : BFB66
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB66

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122018WMA.M
Title : VOC Analysis
Last Update : Fri Dec 28 00:46:50 2018

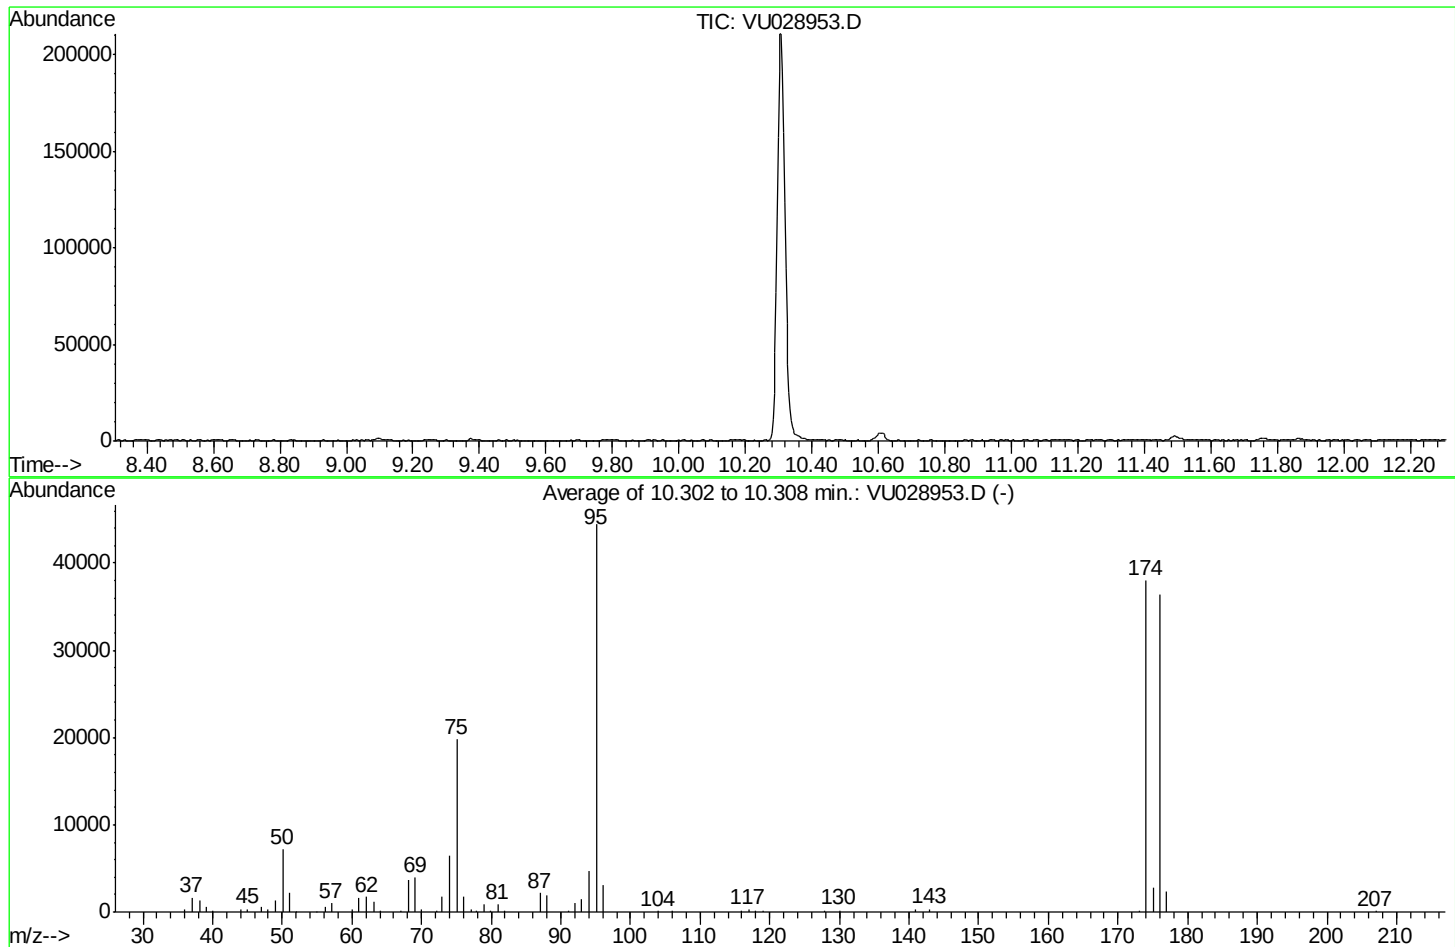

AutoFind: Scans 2839, 2840, 2841; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	7190	PASS
75	95	30	80	44.4	19749	PASS
95	95	100	100	100.0	44440	PASS
96	95	5	9	6.9	3084	PASS
173	174	0.00	2	0.3	96	PASS
174	95	50	120	85.5	38005	PASS
175	174	5	9	7.5	2850	PASS
176	174	95	101	95.7	36389	PASS
177	176	5	9	6.6	2395	PASS

m/z	Abundance
36.10	281.0
37.10	1660.0
38.10	1432.0
39.00	477.0
44.10	420.0
45.10	343.0
47.00	553.0
48.00	232.0
49.10	1325.0
50.10	6889.0
51.10	2210.0
52.00	101.0
56.10	475.0
57.10	928.0
60.00	305.0
61.10	1526.0
62.10	1623.0
63.10	1135.0
64.00	140.0
67.10	123.0
68.10	3484.0
69.10	3886.0
70.00	289.0
72.10	186.0
73.00	1518.0
74.10	6337.0
75.10	18768.0
76.10	1707.0
77.00	274.0
77.90	166.0
79.00	793.0
79.90	207.0
81.00	848.0
81.90	123.0
87.00	2167.0
88.00	1832.0
91.00	106.0
92.10	1029.0
93.00	1443.0
94.10	4470.0
95.10	41552.0
96.10	2898.0
104.10	143.0
106.00	141.0
115.90	160.0
117.00	224.0
117.90	144.0
119.00	171.0
127.80	103.0
130.10	142.0
141.00	273.0
142.90	377.0
173.00	289.0
174.00	34872.0
175.00	2748.0
176.00	33120.0
177.00	2252.0
207.00	116.0

Instrument :
MSVOA_U
ClientSampleId :
BFB66

m/z	Abundance
36.00	356.0
37.10	1713.0
38.10	1449.0
39.00	564.0
40.00	114.0
44.10	420.0
45.10	344.0
47.00	527.0
47.90	253.0
49.10	1426.0
50.10	7459.0
51.10	2330.0
55.00	100.0
56.10	542.0
57.10	1002.0
60.00	309.0
61.10	1643.0
62.10	1814.0
63.10	1249.0
64.00	156.0
67.10	142.0
68.10	3908.0
69.10	4075.0
70.00	273.0
72.10	208.0
73.00	1767.0
74.10	6730.0
75.10	20320.0
76.10	1752.0
77.10	294.0
78.00	167.0
79.00	859.0
80.00	168.0
81.00	882.0
81.90	121.0
87.00	2214.0
88.00	1937.0
91.10	117.0
92.10	1134.0
93.00	1591.0
94.10	4955.0
95.10	45944.0
96.10	3184.0
104.00	153.0
105.90	135.0
115.90	167.0
117.00	272.0
117.90	146.0
118.90	198.0
127.90	105.0
130.00	155.0
141.00	313.0
142.90	353.0
174.00	39112.0
175.00	2916.0
176.00	37544.0
177.00	2475.0
207.00	104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB66

m/z	Abundance
36.00	384.0
37.00	1559.0
38.10	1293.0
39.10	622.0
40.00	160.0
44.10	404.0
45.00	328.0
47.00	494.0
47.90	243.0
49.10	1369.0
50.10	7223.0
51.10	2228.0
54.90	109.0
56.10	596.0
57.10	1023.0
60.10	303.0
61.00	1668.0
62.10	1782.0
63.10	1272.0
64.00	170.0
66.90	128.0
68.10	3828.0
69.10	3837.0
70.00	259.0
72.10	201.0
73.00	1841.0
74.10	6383.0
75.10	20160.0
76.10	1695.0
77.10	262.0
78.00	147.0
79.00	848.0
80.00	193.0
81.00	904.0
81.90	108.0
87.00	2045.0
88.00	1916.0
91.10	121.0
92.10	1091.0
93.00	1563.0
94.10	4892.0
95.10	45824.0
96.10	3171.0
104.00	145.0
105.80	148.0
115.90	151.0
116.90	296.0
117.90	129.0
118.90	189.0
127.90	112.0
130.00	154.0
141.00	381.0
143.00	309.0
174.00	40032.0
175.00	2887.0
176.00	38504.0
177.00	2458.0
207.00	111.0

Instrument :
MSVOA_U
ClientSampleId :
BFB66

m/z	Abundance
44.00	179.0

Instrument :
MSVOA_U
ClientSampleId :
BFB66