


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU122719\
Data File : VU036349.D
Acq On : 27 Dec 2019 11:14
Operator : JC/MD
Sample : BFB33
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB33

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM122719WMA.M
Title : VOC Analysis
Last Update : Mon Dec 30 06:39:20 2019

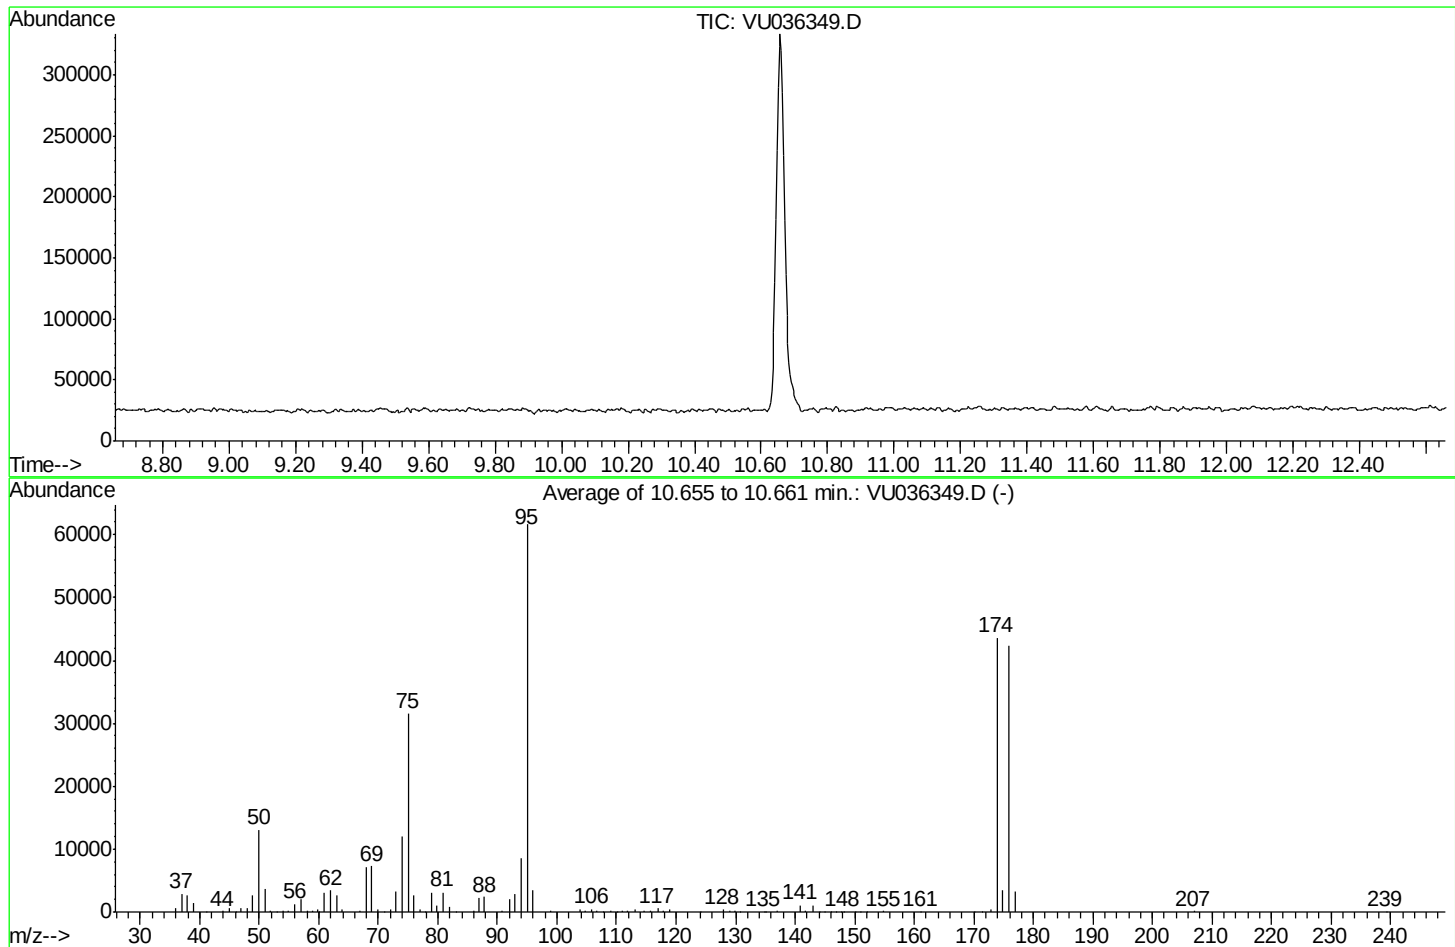

AutoFind: Scans 2897, 2898, 2899; Background Corrected with Scan 2885

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	13092	PASS
75	95	30	80	51.1	31530	PASS
95	95	100	100	100.0	61646	PASS
96	95	5	9	5.5	3414	PASS
173	174	0.00	2	1.0	434	PASS
174	95	50	120	70.8	43658	PASS
175	174	5	9	8.0	3487	PASS
176	174	95	101	96.9	42296	PASS
177	176	5	9	7.6	3217	PASS

m/z	Abundance
37.90	244.0
39.00	763.0
39.90	420.0
41.00	1446.0
41.90	610.0
43.00	2124.0
43.90	2678.0
45.10	216.0
50.00	136.0
50.80	166.0
53.00	348.0
54.10	140.0
55.00	1528.0
56.00	777.0
57.00	1608.0
58.10	211.0
58.90	159.0
60.00	249.0
65.10	195.0
65.90	118.0
67.00	455.0
67.90	325.0
69.00	790.0
70.00	627.0
71.00	944.0
73.10	157.0
73.70	113.0
77.00	246.0
77.80	179.0
78.90	227.0
81.00	395.0
82.00	302.0
83.10	667.0
84.00	436.0
85.00	785.0
90.90	333.0
92.90	239.0
94.10	150.0
95.00	335.0
96.00	381.0
97.00	735.0
98.00	421.0
104.90	110.0
113.20	193.0
119.00	105.0
120.90	101.0
123.00	106.0
126.80	102.0
127.10	109.0
131.00	106.0
267.20	117.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33

m/z	Abundance
35.90	589.0
36.90	2886.0
38.00	2873.0
38.90	2042.0
39.90	277.0
41.00	1306.0
42.00	496.0
42.90	1930.0
43.90	2735.0
45.00	995.0
46.00	107.0
46.80	721.0
47.90	493.0
48.90	2727.0
50.00	12877.0
51.00	3901.0
52.00	175.0
53.00	410.0
54.00	314.0
55.00	1805.0
56.00	2048.0
57.00	3741.0
58.00	534.0
58.90	349.0
59.80	663.0
60.90	2938.0
62.00	3272.0
63.00	2616.0
64.00	298.0
66.00	132.0
66.90	547.0
68.00	7295.0
68.90	7815.0
70.00	996.0
71.00	1139.0
72.00	510.0
73.00	3436.0
74.00	11791.0
75.00	31384.0
76.00	2516.0
77.00	580.0
78.00	305.0
78.90	3463.0
79.90	1131.0
80.90	3667.0
81.90	1046.0
83.10	747.0
83.90	365.0
85.10	605.0
86.00	154.0
86.90	2118.0
87.90	2401.0
90.90	548.0
92.00	2237.0
93.00	3224.0
94.00	8620.0
95.00	61000.0
96.00	3719.0
97.00	660.0
97.90	396.0
99.10	151.0
103.90	417.0
104.80	232.0
105.90	471.0
106.80	180.0
107.60	130.0
109.00	186.0
110.20	136.0
110.90	174.0
111.90	129.0
113.00	534.0
114.70	325.0
115.70	300.0
116.90	635.0
117.80	290.0
118.80	481.0
124.00	133.0
126.90	119.0
128.00	389.0
128.90	227.0
129.90	195.0
130.80	114.0
134.80	201.0
136.90	317.0
140.90	1034.0
141.70	121.0
142.90	974.0
144.90	103.0
146.80	123.0
147.80	134.0
152.00	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33

154.80	162.0
170.10	167.0
171.40	101.0
172.90	388.0
173.90	43416.0
174.90	3500.0
176.00	42056.0
176.90	3238.0
207.10	129.0
239.20	142.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33

m/z	Abundance
35.90	573.0
36.90	3006.0
38.00	2870.0
38.90	2307.0
39.90	284.0
41.00	1576.0
41.90	440.0
43.00	1905.0
44.00	2857.0
45.00	975.0
46.90	684.0
47.90	546.0
48.90	2676.0
50.00	13661.0
51.00	3971.0
51.90	137.0
53.00	330.0
54.00	426.0
54.90	1627.0
56.00	2083.0
57.00	3703.0
58.00	481.0
59.00	337.0
59.80	750.0
60.90	3098.0
62.00	3480.0
62.90	2852.0
63.90	345.0
66.00	137.0
66.90	725.0
67.90	7481.0
68.90	8408.0
70.00	1019.0
71.00	1018.0
72.00	480.0
73.00	3441.0
74.00	12595.0
75.00	32000.0
76.00	2679.0
77.00	675.0
77.80	243.0
78.90	3422.0
79.90	1112.0
80.90	3551.0
81.90	1103.0
83.10	733.0
83.90	365.0
85.10	590.0
86.00	181.0
87.00	2100.0
87.80	2442.0
90.80	461.0
92.00	2049.0
92.90	3105.0
94.00	8920.0
95.00	63712.0
96.00	3800.0
97.00	691.0
97.90	397.0
98.90	177.0
103.80	459.0
104.80	226.0
105.90	477.0
106.70	193.0
107.70	143.0
109.00	154.0
110.20	145.0
110.90	136.0
111.90	204.0
113.10	580.0
114.70	247.0
115.70	301.0
116.90	638.0
117.90	331.0
118.90	419.0
127.00	199.0
128.00	372.0
129.00	160.0
129.90	282.0
130.80	108.0
135.00	133.0
136.90	343.0
140.90	1135.0
141.70	143.0
142.90	1118.0
146.80	148.0
148.10	121.0
150.00	104.0
152.00	118.0
154.80	210.0
170.10	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33

172.90	415.0
173.90	45040.0
174.90	3625.0
176.00	43456.0
176.90	3367.0
207.00	110.0
239.20	109.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33

m/z	Abundance
35.90	547.0
37.00	2941.0
38.00	2927.0
38.90	2429.0
39.90	300.0
41.00	1751.0
41.90	516.0
43.00	1812.0
44.00	2932.0
45.00	836.0
46.90	589.0
47.90	545.0
49.00	2717.0
49.90	13148.0
51.00	3785.0
51.80	134.0
53.00	319.0
54.00	414.0
54.90	1538.0
56.00	1949.0
57.00	3579.0
58.00	436.0
59.00	268.0
60.00	781.0
61.00	3109.0
62.00	3388.0
62.90	2747.0
63.90	307.0
64.90	121.0
66.80	752.0
67.90	7413.0
68.90	7935.0
69.90	1059.0
71.00	979.0
72.00	393.0
73.00	3188.0
74.00	11897.0
75.00	31208.0
75.90	2873.0
77.00	622.0
77.80	213.0
78.80	3250.0
79.90	1023.0
80.80	3412.0
82.00	1031.0
83.10	643.0
83.90	325.0
85.10	646.0
86.00	197.0
87.00	2231.0
87.90	2277.0
90.80	407.0
91.90	1681.0
92.90	2864.0
94.00	8593.0
95.00	61232.0
96.00	3866.0
97.00	608.0
97.90	376.0
98.90	243.0
103.80	470.0
104.80	206.0
105.90	442.0
106.70	214.0
109.10	171.0
110.90	180.0
111.90	270.0
113.10	405.0
114.70	108.0
115.80	302.0
116.90	523.0
117.90	308.0
118.90	357.0
127.10	221.0
127.90	341.0
129.00	138.0
129.80	293.0
130.80	113.0
137.00	247.0
140.90	1040.0
141.70	154.0
142.90	1056.0
144.10	101.0
146.10	189.0
148.10	161.0
150.00	123.0
151.00	114.0
154.90	226.0
161.10	101.0
171.20	112.0
173.00	499.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33

173.90	42520.0
174.90	3338.0
175.90	41376.0
176.90	3047.0
207.00	107.0
267.00	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33